

2011

Measuring Instruments For Velocity







m/s

m³/h

°C

%RH

hPa

CO₂

Lux

СО

rpm







V

mA



Information

Velocity Measurement Engineering


Measurement and application ranges of the velocity probes

Probe selection

The flow measuring range 0 to 100 m/s can be divided into three sections:

- Low-speed velocity 0 to 5 m/s
- Mid-speed velocity 5 to 40 m/s
- High-speed velocity 40 to 100 m/s.


Thermal probes are used for accurate measurements in the range 0 to 5 m/s. Vane probes are ideal for velocities ranging from 5 to 40 m/s. The measuring range of the Pitot tube depends on the differential pressure probe used. The new 100 Pa probe can therefore be used for the exact measurement of flow speed from approx. 1 m/s to 12 m/s. The Pitot tube yields optimum results in the higher velocity range. An additional criterion when selecting the right velocity probe is the temperature. Thermal sensors can normally be used at up to approx. +70 °C. Special design vane probes can be used to max. +350 °C. Pitot tubes are used for temperatures above +350 °C.

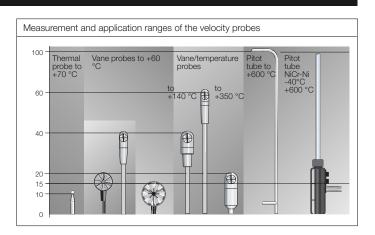

Thermal probes

Thermal probes

The principle of the thermal probe is based on a heated element from which heat is extracted by the colder impact flow. Temperature is kept constant via a regulating switch. The controlling current is directly proportional to the velocity. When thermal velocity probes are used in turbulent flows, the measured result is influenced by the flows impacting the heated body from all directions. In turbulent flows, a thermal velocity sensor indicates higher measured values than a vane probe. This can be observed especially during measurements in ducts. Depending on the design of the duct, turbulent flows can occur even at low velocities.



Thermal hot wire probe for measuring velocity, with direction recognition function

Vane probes

Vane probes

The measuring principle of the vane probe is based on the conversion of a rotation into electric signals. The flowing agent makes the vane rotate. An inductive proximity switch "counts" the revolutions of the vane and supplies a pulse sequence which is converted in the measuring instrument and is then indicated as a velocity value. Large diameters (Ø 60 mm, Ø 100 mm) are suitable for the measurement of turbulent flows (e.g. at outlet ducts) at smaller or medium velocities. Small diameters are more suitable for measurements in ducts; in which case the duct crosssection must be 100 times bigger than the probe cross-section being impacted.

The 16mm probe has proven to be very versatile. It is large enough to have good starting qualities and is small enough to withstand velocities of up to 60 m/s.




Pitot tube

Pitot tube

The Pitot tube opening takes on total pressure and conducts it to connection (a) in the pressure probe. The pure static pressure is taken up by a lateral slot and conducted to connection (b). The resulting differential pressure is a dynamic flow-dependent pressure which is then analysed and indicated


As with thermal probes, the Pitot tube is more likely to react to turbulent flows than a vane probe. Therefore, a free inlet and outlet path must also be ensured during Pitot tube measurements.



Velocity in m/s

S Pitot tube factor

Air density in kg/m³ Differential pressure in Pascal measured at Pitot tube



Measuring volume flow with a funnel


$$v \left[m^3/h \right] = x \left[m/s \right] * 22$$

Volume flow

Velocity

22 Funnel factor

testovent is available for exhaust air (testovent 410 and 415, see ill. right), and for air input (testovent 417, the funnel set for plate inlets and funnels).







Contents

Measuring instrum	ents	
Practical measuring instruments	for velocity	Page
testo 405	Pocket size thermal anemometer	4
testo 410-1/-2	Pocket size vane anemometer	4
testo 416	Compact Vane Anemometer	5
testo 417	Large-Area Vane Anemometer	6
testo 425	Compact Thermal Anemometer	7
testo 435-1/-2/-3/-4	All-rounder for ventilation and indoor air quality	8
testo 521-1	Pitot tube reference instrument	12
testo 521-2	Reference service instrument for Pitot tube measurement	12
testo 512	Pressure and flow velocity measuring instrument	14
Mini wind tunnel	Mini wind tunnel	15
Accessories		
Testo fast printer	Universal infrared printer for differential pressure measuring instrument testo 512	Page 15
ComSoft 3 - Professional	Professional Software including Data Filing	Page 16
Ethernet adapter	Access Ethernet with Testo measuring instruments	Page 18
Measurement syste	ems	
testo 445	Service instrument for ventilation/air conditioning systems	Page 19
testo 400	The reference measuring instrument for A/C and ventilation systems	Page 24

testo 405 is a thermal anemometer with a telescopic handle (max. extension length: 300 mm). It facilitates the measurement of air flow, volume flow and temperature.


testo 405; thermal anemometer with duct holder, holding clip, battery included

Part no.

0560 4053

Pocket size thermal anemometer

- Volume flow calculation up to 99,990 m3/h
- Temperature measurement
- Ideal for measurements in ducts
- Telescopic handle to 300 mm

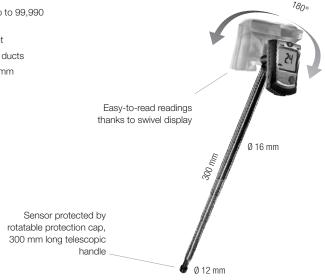

Technical data			
Meas. range	0 to 5 m/s (-20 to 0 °C) 0 to 10 m/s (0 to +50 °C) -20 to +50 °C 0 to +99990 m³/h	Oper. temp.	0 to +50 °C
		Storage temp.	-20 to +70 °C
		Battery type	3 batteries Type AAA
Accuracy	±(0.1 m/s + 5% of mv)	Battery life	Approx. 20 h
$\begin{array}{ll} \pm 1 \text{ digit} & (0 \text{ to } +2 \text{ m/s}) \\ & \pm (0.3 \text{ m/s} +5\% \text{ of mv}) \\ & \text{(remaining range)} \\ & \pm 0.5 \text{ °C} \end{array}$	±(0.3 m/s + 5% of mv)	Weight	115 g (with batteries, without packaging)
	(0 0 /	Warranty	2 years
Resolution	0.01 m/s 0.1 °C		

Accessories	Part no.
testovent 410, volume flow funnel, Ø 340 mm/330x330 mm, incl. case	0554 0410
testovent 415, volume flow funnel, Ø 210 mm/210x210 mm, incl. case	0554 0415
ISO calibration certificate velocity two point calibration; calibration points 5m/s and 10m/s	0520 0094
ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s	0520 0004

testo 410-1/-2

testo 410-1 measures air speed and temperature. It is ideal for quick spot checks at air outlets on account of its integrated measurement with the 40mm vane. Timed mean calculation is possible.

In addition to air speed and temperature, testo 410-2 also measures air moisture. Testo's very own, patented humidity sensor guarantees accurate readings. In this way, air conditions can be reliably checked.

Pocket size vane anemometer

- Flow velocity measuring instrument with temperature measurement
- Integrated measurement with 40 mm vane
- Timed mean value calculation
- Hold function and max./min. values
- Windchill calculation for outside areas (perceived temperature)
- Display illumination

testo 410-1; vane anemometer with built-in NTC air thermometer, incl protective cap, batteries and calibration protocol

Part no.

0560 4101

- Protective cap for safe storage
- Including wrist strap, belt holder and calibration protocol

Additional advantages of testo 410-2

- Air humidity measurement with longterm stable Testo humidity sensor
- Incl. dewpoint calculation and wet bulb

testo 410-2; vane anemometer with integrated humidity measurement and NTC air thermometer, incl protective cap, batteries and calibration protocol

Part no.

0560 4102



Technical data				
	testo 410-1/-2		testo 410-2	
Probe type	Vane	NTC	Testo humid. sensor, cap.	
Meas. range	0.4 to 20 m/s	-10 to +50 °C	0 to 100 %RH	
Accuracy ±1 digit	\pm (0.2 m/s + 2% of mv)	±0.5 °C	±2.5 %RH (5 to 95 %RH)	
Resolution	0.1 m/s	0.1 °C	±0.1 %RH	
Battery life	100 h (average, without display illumination)		60 h (average, without display illumination)	

Common Techr	nical Data testo 410-1/
Dimensions	133 x 46 x 25 mm (incl. protective cap)
Oper. temp.	-10 to +50 °C
Storage temp.	-20 to +70 °C
Protection class	IP10

Battery type	2 batteries Type AAA
Weight	110 g (with protective cap and batteries)
Measuring rate	0.5 s
Warranty	2 years

Accessories	Part no.
ISO calibration certificate velocity two point calibration; calibration points 5m/s and	0520 0094 0m/s
ISO calibration certificate/Velocity hot wire, vane anemometer, Pitot tube; calibration	0520 0034 oints 5; 10; 15; 20 m/s



The compact testo 416 anemometer with permanently attached vane probe with telescopic handle (max. 890mm).

Volume flow is shown directly in the display. Accurate volume flow calculation due to easy input of duct area.

Timed and multi-point mean calculation provide information on mean volume flow.

Min/max values can also be shown in the display. The Hold function enables you to freeze the current reading in the display.

testo 416, vane anemometer with permanently attached 16 mm telescopic vane (max. 890 mm), with battery and calibration protocol

Part no.

0560 4160

Compact Vane Anemometer

- Direct display of volume flow
- Multi-point or timed mean calculation
- Max/min values
- Hold button to freeze readings
- Display light
- Auto-Off function
- TopSafe, instrument protection against dirt and knocks (optional)



Accessories	Part no.
Case for measuring instrument and probes	0516 0210
TopSafe, protects from impact and dirt	0516 0221
Transport case for meas. instr. and probes (405 x 170 x 85 mm)	0516 0201
Recharger for 9V rechargeable battery for external recharging of 0515 0025 battery	0554 0025
9V rech. battery for instrument instead of battery	0515 0025
ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s	0520 0024
ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s $$	0520 0004
ISO calibration certificate/Velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s	0520 0034

Technical data			
Probe type	Vane	Oper. temp.	-20 to +50 °C
Meas. range	+0.6 to +40 m/s	Storage temp.	-40 to +85 °C
Accuracy	\pm (0.2 m/s +1.5% of mv)	Battery type	9V block battery, 6F22
±1 digit		Battery life	80 h
Resolution	0.1 m/s	Dimensions	182 x 64 x 40 mm
		Weight	325 g
		Material/Housing	ABS
		Warranty	2 years

The compact testo 417 anemometer with built-in flow/temperature vane Ø 100 mm to measure flow speed, volume flow and temperature.

Volume flow is shown directly in the display. Accurate volume flow calculation thanks to easy input of duct area. In addition, it is easy to switch to the current temperature reading.

The flow direction, i.e. drawn in or blowing, is visible in the display.

Timed and multi-point mean calculation provide information on mean volume flow, flow speed and temperature readings.

The optional funnel set facilitates efficient measurements at ventilator grilles and disc outlets.

Min/max values can also be shown in the display. Current readings can be frozen in the display using the Hold function.

testo 417, vane anemometer with built-in 100 mm vane, incl. temperature measurement, battery and calibration protocol

Part no.

0560 4170

Large-Area Vane Anemometer

- Direction of flow recognition
- Temperature, flow and volume flow measurement
- Multi-point and timed mean calculation
- Max/min values
- Hold button to freeze readings
- Display light
- Auto Off function

Built-in Ø 100 mm vane



Technical data			
Probe type	NTC	Vane	Volume flow
Meas. range	0 to +50 °C	+0.3 to +20 m/s	0 to +99999 m³/h
Accuracy ±1 digit	±0.5 °C	±(0.1 m/s +1.5% of mv)	
Resolution	0.1 °C	0.01 m/s	0.1 m ³ /h (0 to +99.9 m ³ /h) 1 m ³ /h (+100 to +99999 m ³ /h)

Oper. temp.	0 to +50 °C
Storage temp.	-40 to +85 °C
Battery type	9V block battery, 6F22
Battery life	50 h

Dimensions	277 x 105 x 45 mm
Weight	230 g
Material/Housing	ABS
Warranty	2 years

Accessories	Part no.
Case for measuring instrument and probes	0516 0210
Funnel set consisting of funnel for disc outlets (Ø 200) and funnel for ventilator (330 x 330 mm) for in- and outgoing air	0563 4170
Recharger for 9V rechargeable battery for external recharging of 0515 0025 battery	0554 0025
9V rech. battery for instrument instead of battery	0515 0025
DAkkS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s	0520 0244
ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s	0520 0004
ISO calibration certificate/Velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s	0520 0034
ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s	0520 0024

*Successor organization of the DKD



The compact testo 425 anemometer with permanently attached thermal flow probe (probe head Ø 7.5 mm) incl. telescopic handle.

Volume flow is shown directly in the display. Accurate volume flow calculation thanks to easy input of duct area. In addition, it is also possible to switch to the current temperature reading.

Timed and multi-point mean calculation provide information on mean volume flow, flow speed and temperature reading.

Min/max values can also be shown in the display. The Hold function makes it possible to freeze current readings in the display.

testo 425, thermal anemometer with permanently attached flow probe (Ø probe head 7.5 mm), incl. temperature measurement and telescopic handle (max. 820 mm), battery and calibration protocol

Part no.

0560 4251

Compact Thermal Anemometer

- Temperature, flow and volume flow measurement
- Multi-point and timed mean calculation
- Max/min values
- Hold button to freeze readings
- Display light
- Auto Off function
- TopSafe, the indestructible protective case (optional)



Accessories	Part no.
Case for measuring instrument and probes	0516 0210
TopSafe, protects from impact and dirt	0516 0221
Transport case for meas. instr. and probes (405 x 170 x 85 mm)	0516 0201
Recharger for 9V rechargeable battery for external recharging of 0515 0025 battery	0554 0025
9V rech. battery for instrument instead of battery	0515 0025
ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s $$	0520 0004
ISO calibration certificate/Velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s $$	0520 0034

Probe type	Thermal		NTC		
Meas. range	0 to +20 m/s		-20 to +7	O °C	
Accuracy ±1 digit	±(0.03 m/s +5% of mv)	±(0.03 m/s +5% of mv)		±0.5 °C (0 to +60 °C) ±0.7 °C (remaining range)	
Resolution	0.01 m/s		0.1 °C		
Oper. temp.	-20 to +50 °C	Dimen	sions	182 x 64 x 40 mm	

Oper. temp.	-20 to +50 °C	- 1
Storage temp.	-40 to +85 °C	١
Battery type	9V block battery, 6F22	- 1
Rattony life	20 h	١

Dimensions	182 x 64 x 40 mm
Weight	285 g
Material/Housing	ABS
Warranty	2 years

All measurement parameters for air conditioning

testo 435 provides the possibility of analysing indoor air. On the one hand, this serves as an indicator for the well-being of people at their workplaces, and on the other hand as an important and deciding factor in storage and production processes.

In addition to this, Indoor Air Quality signals whether the air conditioning system (HVAC) is working with as much energy economy as possible, or whether it needs to be adjusted with the help of testo 435.

The parameters CO₂, relative humidity and room temperature are available for evaluating the quality of the air. Absolute pressure, draught, Lux, U-value and surface temperature can additionally be determined. In order to determine volume flow, all the possibilities of flow velocity measurement are available, such as thermal probes, vane anemometers and Pitot tubes.

Versatility with wireless probes

In addition to classical probes on wires, a wireless measurement up to a distance of 20 m (without obstruction) is possible. Damage to the wire or hindrances in usage are thus eliminated. A maximum of three wireless probes can be recorded and displayed with testo 435. The wireless probes are for the measurement parameters temperature and, depending on the instrument type, humidity. The optional, easily plugged-in radio module can be retrofitted at any time.

All-rounder for ventilation and Indoor Air Quality

Common product advantages testo 435

- Wide selection of probes:
 - IAQ probe for evaluating indoor air quality via CO₂, air temperature, indoor air humidity and absolute pressure
 - Thermal probes with integrated temperature and air humidity measurement
 - Vane and hot wire probes
 - Radio probes for temperature
- Easy operation with user profiles
- Printout on the testo fast printer

Further product advantages of the variants

- Integrated differential pressure measurement (435-3/-4, not retrofittable)
 - for flow measurement
 - for monitoring filters
- Extended instrument function (435-2/-4, not retrofittable)
 - Instrument store for 10,000 readings and up to 99 measurement sites
 - PC software for analysing, archiving and documenting measurement data
 - Humidity probes with radio or wire
 - Lux probe connection possible
 - Comfort level probe connection possible
 - U-value probe connection possible



testo 435-

testo 435-1, multi-functional meas. instr., for A/C, ventilation and Indoor Air Quality, with battery and calibration protocol

Part no. **0560 4351**

testo 435-2

testo 435-2, multi-functional measuring instrument for A/C, ventilation and Indoor Air Quality with readings memory, PC software and USB data transmission cable, incl. battery and calibration protocol

Part no. **0563 4352**

testo 435-3

testo 435-3, multi-functional measuring instrument with built-in differential pressure measurement for air conditioning, ventilation and Indoor Air Quality, with battery and calibration protocol

Part no. **0560 4353**

testo 435-4

testo 435-4, multi-functional meas. instr. with built-in differential pressure measurement for A/C, ventilation and Indoor Air Quality with readings memory, PC software and USB data transmission cable, with battery and calibration protocol

Part no. **0563 4354**



435-1/-2/-3/-4

Pitot tube, 1000 mm long

Probes

435-1/-2/-3/-4							
IAQ probes	Illustration			Meas. range	Accuracy		Part no.
IAQ probe to assess Indoor Air Quality, CO ₂ , humidity, temperature and absolute pressure measurement, with desk-top stand				0 to +50 °C 0 to +100 %RH 0 to +10000 ppm CO ₂ +600 to +1150 hPa	±0.3 °C ±2 %RH (+2 to +98 %RH) ±(50 ppm CO ₂ ±2% of mv) (0 to +5000 pp ±(100 ppm CO ₂ ±3% of mv) (+5001 to +10 ±3 hPa	m CO ₂) 0000 ppm	0632 1535 co ₂)
Ambient CO probe, for detecting CO in buildings and rooms	3			0 to +500 ppm C0	±5% of mv (+100.1 to +500 ppm C ±5 ppm C0 (0 to +100 ppm C0)	(0)	0632 1235
Flow velocity probes	Illustration			Meas. range	Accuracy		Part no.
Thermal velocity probe with built-in temperature and humidity measurement, Ø 12 mm, with elescopic handle (max. 745 mm)	4			-20 to +70 °C 0 to +100 %RH 0 to +20 m/s	±0.3 °C ±2 %RH (+2 to +98 %RH) ±(0.03 m/s +4% of mv)		0635 1535
rane meas. probe, 16 mm diameter, with elescopic handle max. 890 mm, e.g. for meas. in lucts, can be used from 0 to +60 °C		(+\$)		+0.6 to +40 m/s Oper. temp. 0 to +60 °C	±(0.2 m/s +1.5% of mv)		0635 9535
fane meas. probe, 60 mm diameter, with elescopic handle max. 910 mm, e.g. for meas. at luct exit, can be used from 0 to +60 °C	(+0.25 to +20 m/s Oper. temp. 0 to +60 °C	±(0.1 m/s +1.5% of mv)		0635 9335
on the form of the	4	·		0 to +20 m/s -20 to +70 °C	±(0.03 m/s +5% of mv) ±0.3 °C (-20 to +70 °C)		0635 1025
Funnel measurement	Illustration			Meas. range	Accuracy		Part no.
/ane meas. probe, 100 mm diameter, for measurements with funnel set 0563 4170	-			+0.3 to +20 m/s 0 to +50 °C	$\pm (0.1 \text{ m/s} +1.5\% \text{ of mv})$ $\pm 0.5 ^{\circ}\text{C}$		0635 9435
Funnel set consisting of funnel for disc outlets (Ø 20 or ventilator (330 x 330 mm) for in- and outgoing a		1 🐠					0563 4170
Absolute pressure probes	Illustration			Meas. range	Accuracy		Part no.
Absolute pressure probe 2000 hPa				0 to +2000 hPa	±5 hPa		0638 1835
Air probes	Illustration			Meas. range	Accuracy	t99	Part no.
ifficient, robust NTC air probe	(6)	115 mm	50 mm	-50 to +125 °C	±0.2 °C (-25 to +80 °C) ±0.4 °C (remaining range)	60 s	0613 1712
		Ø 5 mm	Ø 4 mm			Conn.:	Fixed cable 1.2 m
Surface probes	Illustration			Meas. range	Accuracy	t99	Part no.
ast-reaction paddle surface probe, for measureme i inaccessible places, e.g. narrow apertures and sli C Type K		145 mm Ø 8 mm	40 mm	0 to +300 °C	Class 2*	5 s Conn.:	0602 0193 Fixed cable
ast-action surface probe with sprung thermocouple				-60 to +300 °C			0602 0393
	4.7	115 mm		-00 10 +300 *6	Class 2*	3 s	0002 0000
trip, also for uneven surfaces, measurement range	0	0 5 mm	Ø 12 mm	-60 (0 +300 °C	Class 2*		
rip, also for uneven surfaces, measurement range nort-term to +500°C, TC Type K			Ø 12 mm		Class 2*	Conn.:	Fixed cable 0602 4592
trip, also for uneven surfaces, measurement range nort-term to +500°C, TC Type K ipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range	Proceedings		Ø 12 mm	-60 to +130 °C			Fixed cable
rip, also for uneven surfaces, measurement range nort-term to +500°C, TC Type K ipe wrap probe for pipe diameter 5 to 65 mm, rith exchangeable measuring head. Meas. range hort-term to +280°C, TC Type K	Processing		Ø 12 mm	-60 to +130 °C	Class 2*	Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable
trip, also for uneven surfaces, measurement range hort-term to +500°C, TC Type K ripe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range hort-term to +280°C, TC Type K clamp probe for measurements on pipes, pipe liameter 15 to 25 mm (max. 1"), meas. range	• • • • • • • • • • • • • • • • • • •		Ø 12 mm			Conn.: 5 s	Fixed cable 0602 4592
trip, also for uneven surfaces, measurement range nort-term to +500°C, TC Type K lipe wrap probe for pipe diameter 5 to 65 mm, rith exchangeable measuring head. Meas. range hort-term to +280°C, TC Type K lamp probe for measurements on pipes, pipe iameter 15 to 25 mm (max. 1"), meas. range hort-term up to +130°C, TC Type K			Ø 12 mm	-60 to +130 °C	Class 2*	Conn.: 5 s Conn.: 5 s	Fixed cable 0602 4592 Fixed cable
trip, also for uneven surfaces, measurement range hort-term to +500°C, TC Type K lipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range hort-term to +280°C, TC Type K clamp probe for measurements on pipes, pipe liameter 15 to 25 mm (max. 1"), meas. range hort-term up to +130°C, TC Type K Immers./penetr. probes	Illustration		Ø 12 mm	-60 to +130 °C -50 to +100 °C Meas. range	Class 2* Class 2* Accuracy	Conn.: 5 s Conn.: 5 s Conn.: t99	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no.
trip, also for uneven surfaces, measurement range hort-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe liameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Vaterproof immersion/penetration probe,		0 5 mm		-60 to +130 °C -50 to +100 °C	Class 2*	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable
trip, also for uneven surfaces, measurement range hort-term to +500°C, TC Type K Tipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range hort-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe liameter 15 to 25 mm (max. 1"), meas. range hort-term up to +130°C, TC Type K Immers./penetr. probes Vaterproof immersion/penetration probe,	Illustration	0 5 mm		-60 to +130 °C -50 to +100 °C Meas. range	Class 2* Class 2* Accuracy	Conn.: 5 s Conn.: 5 s Conn.: 7 s	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no.
ctrip, also for uneven surfaces, measurement range chort-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, TC Type K	Illustration	0 5 mm		-60 to +130 °C -50 to +100 °C Meas. range	Class 2* Class 2* Accuracy	Conn.: 5 s Conn.: 5 s Conn.: 7 s	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293
trip, also for uneven surfaces, measurement range hort-term to +500°C, TC Type K lipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range hort-term to +280°C, TC Type K lamp probe for measurements on pipes, pipe liameter 15 to 25 mm (max. 1"), meas. range hort-term up to +130°C, TC Type K Immers./penetr. probes Vaterproof immersion/penetration probe, C Type K	Illustration	0 5 mm		-60 to +130 °C -50 to +100 °C Meas. range	Class 2* Class 2* Accuracy Class 2*	Conn.: 5 s Conn.: 5 s Conn.: 7 s	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293
chort-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, TC Type K 435-2/-4 IAQ probes Comfort level probe for degree of turbulence measurement with telescopic handle (max. 820)	Illustration	0 5 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C	Class 2* Class 2* Accuracy	Conn.: 5 s Conn.: 5 s Conn.: 7 s	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m
trip, also for uneven surfaces, measurement range hort-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe liameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Vaterproof immersion/penetration probe, TC Type K 435-2/-4 IAQ probes Comfort level probe for degree of turbulence neasurement with telescopic handle (max. 820 nm) and stand, meets EN 13779 requirements	Illustration	0 5 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C Meas. range 0 to +50 °C	Class 2* Class 2* Accuracy Class 2* Accuracy ±0.3 °C	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m
chrip, also for uneven surfaces, measurement range whort-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, C Type K IAQ probes Comfort level probe for degree of turbulence measurement with telescopic handle (max. 820 mm) and stand, meets EN 13779 requirements Lux probe, for measuring light intensity	Illustration	0 5 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C Meas. range 0 to +50 °C	Class 2* Class 2* Accuracy Class 2* Accuracy ±0.3 °C ±(0.03 m/s +4% of mv) Accuracy to DIN 5032, Part 6: f1 = 6% = V(Lambda) adjustment	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m Part no. 0628 0109
chort-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, C Type K IAQ probes Comfort level probe for degree of turbulence measurement with telescopic handle (max. 820 mm) and stand, meets EN 13779 requirements Lux probe, for measuring light intensity Humidity probes	Illustration Illustration max. 820 mm	0 5 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C Meas. range 0 to +50 °C 0 to +5 m/s	Class 2* Class 2* Accuracy Class 2* Accuracy ±0.3 °C ±(0.03 m/s +4% of mv) Accuracy to DIN 5032, Part 6: f1 = 6% = V(Lambda) adjustment f2 = 5% = cos-like weighting, Class Accuracy ±0.3 °C	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m Part no. 0628 0109
chort-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, C Type K IAQ probes Comfort level probe for degree of turbulence measurement with telescopic handle (max. 820 mm) and stand, meets EN 13779 requirements Lux probe, for measuring light intensity Humidity probes	Illustration max. 820 mm	0 5 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C Meas. range 0 to +50 °C 0 to +5 m/s	Class 2* Class 2* Accuracy Class 2* Accuracy L0.3 °C L0.03 m/s +4% of mv) Accuracy to DIN 5032, Part 6: f1 = 6% = V(Lambda) adjustment f2 = 5% = cos-like weighting, Class Accuracy	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m Part no. 0628 0109 0635 0545 Part no.
strip, also for uneven surfaces, measurement range short-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, TC Type K 435-2/-4 IAQ probes Comfort level probe for degree of turbulence measurement with telescopic handle (max. 820 mm) and stand, meets EN 13779 requirements Lux probe, for measuring light intensity Humidity probes -lumidity/temperature probe	Illustration max. 820 mm	0.5 mm 50 mm 0.3.7 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C Meas. range 0 to +50 °C 0 to +5 m/s	Class 2* Class 2* Accuracy Class 2* Accuracy ±0.3 °C ±(0.03 m/s +4% of mv) Accuracy to DIN 5032, Part 6: f1 = 6% = V(Lambda) adjustment f2 = 5% = cos-like weighting, Class Accuracy ±0.3 °C	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m Part no. 0628 0109 0635 0545 Part no.
ctrip, also for uneven surfaces, measurement range thort-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, TC Type K IAQ probes Comfort level probe for degree of turbulence measurement with telescopic handle (max. 820 mm) and stand, meets EN 13779 requirements Lux probe, for measuring light intensity Humidity probes	Illustration max. 820 mm	0.5 mm 50 mm 0.3.7 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C Meas. range 0 to +50 °C 0 to +5 m/s	Class 2* Class 2* Accuracy Class 2* Accuracy ±0.3 °C ±(0.03 m/s +4% of mv) Accuracy to DIN 5032, Part 6: f1 = 6% = V(Lambda) adjustment f2 = 5% = cos-like weighting, Class Accuracy ±0.3 °C ±2 %RH (+2 to +98 %RH) Oper. temp.	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m Part no. 0628 0109 0635 0545 Part no. 0636 9735
clarip, also for uneven surfaces, measurement range short-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, TC Type K 435-2/-4 IAQ probes Comfort level probe for degree of turbulence measurement with telescopic handle (max. 820 mm) and stand, meets EN 13779 requirements Lux probe, for measuring light intensity Humidity probes Humidity probes Humidity Probes Humidity Probes Pitot tubes	Illustration Illustration max. 820 mm Illustration	0 5 mm 114 mm 50 mm 0 5 mm 0 3.7 m 0 12 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C Meas. range 0 to +50 °C 0 to +5 m/s	Class 2* Class 2* Accuracy Class 2* Accuracy ±0.3 °C ±(0.03 m/s +4% of mv) Accuracy to DIN 5032, Part 6: f1 = 6% = V(Lambda) adjustment f2 = 5% = cos-like weighting, Class Accuracy ±0.3 °C ±2 %RH (+2 to +98 %RH)	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m Part no. 0628 0109 0635 0545 Part no. 0636 9735
strip, also for uneven surfaces, measurement range short-term to +500°C, TC Type K Pipe wrap probe for pipe diameter 5 to 65 mm, with exchangeable measuring head. Meas. range short-term to +280°C, TC Type K Clamp probe for measurements on pipes, pipe diameter 15 to 25 mm (max. 1"), meas. range short-term up to +130°C, TC Type K Immers./penetr. probes Waterproof immersion/penetration probe, TC Type K 435-2/-4 IAQ probes Comfort level probe for degree of turbulence measurement with telescopic handle (max. 820 mm) and stand, meets EN 13779 requirements Lux probe, for measuring light intensity Humidity probes Humidity probes Humidity/temperature probe 435-3/-4 Prandtl's Pitot tubes Pitot tube, 350 mm long, Ø 7 mm, stainless steel, measures flow speed Pitot tube, 500 mm long	Illustration Illustration max. 820 mm Illustration	0.5 mm 50 mm 0.3.7 mm		-60 to +130 °C -50 to +100 °C Meas. range -60 to +400 °C Meas. range 0 to +50 °C 0 to +5 m/s	Class 2* Class 2* Accuracy Class 2* Accuracy ±0.3 °C ±(0.03 m/s +4% of mv) Accuracy to DIN 5032, Part 6: f1 = 6% = V(Lambda) adjustment f2 = 5% = cos-like weighting, Class Accuracy ±0.3 °C ±2 %RH (+2 to +98 %RH) Oper. temp.	Conn.: 5 s Conn.: 5 s Conn.:	Fixed cable 0602 4592 Fixed cable 0602 4692 Fixed cable Part no. 0602 1293 Fixed cable 1.2 m Part no. 0628 0109 0635 0545 Part no. 0636 9735

0 to +600 °C

0635 2345



435-1/-2/-3/-4

Accessories / Technical data

Technical data								
Probe type	NTC	Туре К	Type T	Testo humid. sensor, cap.	Vane	Hot wire	Absolute pressure probe	CO ₂ (IAQ probe)
Meas. range	-50 to +150 °C	-200 to +1370 °C	-200 to +400 °C	0 to +100 %RH	0 to +60 m/s	0 to+20 m/s	0 to +2000 hPa	0 to +10000 ppm CO ₂
Accuracy ±1 digit	±0.2 °C (-25 to +74.9 °C) ±0.4 °C (-50 to -25.1 °C) ±0.4 °C (+75 to +99.9 °C) ±0.5% of mv (remaining range)	±0.3 °C (-60 to +60 °C) ±(0.2 °C +0.3% of mv) (remaining range)	±0.3 °C (-60 to +60 °C ±(0.2 °C +0.3% of mv) (remaining range)	See probe data	See probe data	See probe data	See probe data	See probe data
Resolution	0.1 °C	0.1 °C	0.1 °C	0.1 %RH	0.01 m/s (60 vane) 0.1 m/s (16 vane)	0.01 m/s	0.1 hPa	1 ppm CO ₂

Technical data	Technical data 435-2/-4				
Probe type	Lux				
Meas. range	0 to +100000 Lux				
Accuracy ±1 digit	See probe data				
Resolution	1 Lux / 0.1 Hz				

Technical data 435-3/-4			
Probe type	Differential pressure probe, internal		
Meas. range	0 to +25 hPa		
Accuracy ±1 digit	±0.02 hPa (0 to +2 hPa) 1% of mv (remaining range)		
Overload	200 hPa		
Resolution	0.01 hPa		

Oper. temp.	-20 to +50 °C
Storage temp.	-30 to +70 °C
Dimensions	220 x 74 x 46 mm
Battery type	Alkali manganese, mignon, Type AA
Battery life	200 h (typical vane measurement)
Weight	450 g
Material/Housing	ABS/TPE/Metal
Warranty	2 years

Accessories		D .
		Part no.
Transport and Protection		
Service case for basic equipment of measuring inst dimensions: 400 x 310 x 96 mm	trument and probes,	0516 0035
Service case for measuring instrument, probe and $520x380x120~mm$	accessories, dimensions	0516 0435
Additional Accessories and Spare Part	ts	
Handle for attachable humidity probe head for conrprobe wire, for measurement / calibration of humid		0430 9735
Lithium battery button cell, CR2032 AA batteries fo	r radio handle	0515 0028
Plug-in mains adapter, 5 VDC 500 mA with Europea 50-60 Hz	an adapter, 100-250 VAC,	0554 0447
testovent 410, volume flow funnel, Ø 340 mm/330	x330 mm, incl. case	0554 0410
testovent 415, volume flow funnel, Ø 210 mm/210	x210 mm, incl. case	0554 0415
Funnel set consisting of funnel for disc outlets (0 2 ventilator (330 x 330 mm) for in- and outgoing air	00) and funnel for	0563 4170
Connection hose, silicone, 5m long, max. load 700 h	Pa (mbar)	0554 0440
testo saline pots for control and humidity adjustmer 11.3 %RH and 75.3 %RH with adapter for humidity calibration of humidity probe		0554 0660
Sintered PTFE filter, \emptyset 12 mm, for corrosive media, (long-term measurements), high flow velocities.	High humidity range	0554 0756
Stainless steel sintered cap, \emptyset 12 mm, is screwed measurements at higher flow velocities or in contar		0554 0647
Adhesive material for fixing and sealing		0554 0761

Accessories	Part no.
Printer and Accessories	
Testo fast printer with wireless infrared interface, 1 roll thermal pap AA batteries, for printing out measurements on site	per and 4 0554 0549
Spare thermal paper for printer (6 rolls), permanent ink, measurem documentation legible for up to 10 years	ent data 0554 0568
Spare thermal paper for printer (6 rolls)	0554 0569
External fast charger for 1-4 AA rech. batteries, incl. 4 Ni-MH rech with individual cell charging and charge control display, incl. impuls charging, integrated discharge function, with built-in international rolug, 100-240 V, 300 mA, 50/60 Hz	e trickle
Calibration Certificates	
SO calibration certificate/temperature, meas. instr. with surface prealibration points $+60^{\circ}$ C; $+120^{\circ}$ C; $+180^{\circ}$ C	obe; 0520 0071
SO calibration certificate humidity, Calibration points 11.3 %RH ar %RH at +25°C	d 75.3 0520 0006
SO calibration certificate/pressure; differential pressure; 5 points over meas. range	listributed 0520 0005
SO calibration certificate velocity, hot wire, vane anemometer; cali points 0.5; 0.8; 1; 1.5 m/s	oration 0520 0024
SO calibration certificate velocity, hot wire, vane anemometer, Pito calibration points 1; 2; 5; 10 m/s	tube; 0520 0004
SO calibration certificate/Velocity, hot wire, vane anemometer, Pito calibration points 5; 10; 15; 20 m/s	t tube; 0520 0034
SO calibration certificate/light, Calibration points 0;500;1000;200 Lux	0;4000 0520 0010
SO calibration certificate/CO2, CO2 probes; calibration points 0; 1 5000 ppm	000; 0520 0033



435-1/-2/-3/-4

Ordering data Option: Radio

435-1/-2/-3/-4 Radio module for upgrading measuring instrument with radio option		
Country versions	Radio freq.	Part no.
Radio module for measuring instrument, 869.85 MHz, approval for the countries: DE, FR, UK, BE, NL, ES, IT, SE, AT, DK, FI, HU, CZ, PL, GR, CH, PT, SI, MT, CY, SK, LU, EE, LT, IE, LV, NO	869.85 MHz FSK	0554 0188
Radio module for measuring instrument, 915.00 MHz FSK, approval for USA, CA, CL	915.00 MHz FSK	0554 0190

Radio handles with probe head for surface measurement	Meas. range	Accuracy	Resolution	t ,		
Radio handle for attachable probe heads with T/C probe head for surface measurement	50 to +350 °C Short-term to +500 °C	Radio handle: $\pm (0.5~^{\circ}\text{C} + 0.3\% \text{ of mv}) \text{ (-40 to +500 °C)} $ $\pm (0.7~^{\circ}\text{C} + 0.5\% \text{ of mv}) \text{ (remaining range)} $ T/C probe head: Class 2	0.1 °C (-50 to +199.9 °C) 1.0 °C (remaining range)	5		
Country versions		Radio freq.	Part no.			
Radio handle for plug-in probe heads, incl. T/C adapter, approval for the countries: DE, FR, UK, HU, CZ, PL, GR, CH, PT, SI, MT, CY, SK, LU, EE, LT, IE, LV, NO	BE, NL, ES, IT, SE, AT, DK, FI,	869.85 MH	lz FSK 0554 0189			
Radio immersion/penetration probes, T/C probe head for surface measurement, attachable to radio handle, T/C Type K 0602 0394						
Radio handle for plug-in probe heads, incl. T/C adapter, approval for USA, CA, CL 915.00 MHz FSK 0554 019						
T/C probe head for surface measurement, attachable to radio handle, T/C Type K			0602 0394			

435-2/-4				
Radio probes incl. humidity probe head	Meas. range	Accuracy		Resolution
Radio handle for attachable probe heads with humidity probe head	0 to +100 %RH -20 to +70 °C	±2 %RH (+2 to + ±0.3 °C	98 %RH)	0.1 %RH 0.1 °C
Country versions			Radio freq.	Part no.
adio handle for plug-in probe heads, incl. T/C adapter, approval for the countries: DE, FR, UK, BE, NL, E T, SI, MT, CY, SK, LU, EE, LT, IE, LV, NO	S, IT, SE, AT, DK, FI, HU, C	Z, PL, GR, CH,	869.85 MHz FSK	0554 0189
lumidity probe head, attachable to radio handle				0636 9736
Radio handle for plug-in probe heads, incl. T/C adapter, approval for USA, CA, CL			915.00 MHz FSK	0554 0191
Humidity probe head, attachable to radio handle				0636 9736

Radio probes: 0	Radio probes: General technical data								
	Radio handle		Measuring rate	leasuring rate 0.5 s or 10 s, adjustable		Unidirectional			
Battery type	2 AAA micro batteries		on handle						
Battery life	215 h (meas. rate 0.5 s)				Oper. temp.	-20 to +50 °C			
	6 months (meas. rate 10 s)			Up to 20 m (without	Storage temp.	-40 to +70 °C			
Protection class	IP54			obstructions)					

testo 521-1 / testo 521-2

 Temp. compensated differential pressure sensor in instrument Additional 2 probe sockets for

Pitot tube reference instrument

The highly accurate differential pressure meter, testo 521, with an internal pressure sensor from 0 to 100 hPa is ideal for Pitot tube measurements in the range 5 to 100 m/s. testo 521 is available in 2 accuracy classes. testo 521-1 with an internal pressure sensor with Class 0.2, testo 521-2 with an internal pressure sensor with Class 0.1.

and volume flow

measuring pressure and temp.

Direct calculation of velocity speed

- Multi-point and timed mean calculation
- Density compensation
- Up to two 4 to 20 mA interfaces connectable to hand-held instr.
- 1 analog signal can be evaluated per interface
- Scaling of analog signal in hand-held instrument
- Transmitter can be supplied with power from testo 521, for example
- 4 to 20 mA interface can be connected to testo 521, 526, 400, 650 und 950 hand-held instruments



Overload Static pressure Zeroing Part no.

The measurement data can be saved according to location and analysed on your PC or printed on site on your Testo fast printer.

In the case of velocity speeds in

the range from 1 to 12 m/s, you

measurements using the 100 Pa

probe which can be attached

can carry out accurate

externally.

testo 521-1, differential pressure meter 0 to 100 hPa incl. battery and calibration protocol

Part no.

0560 5210 Pressure probes

testo 521-2, differential pressure meter 0 to 100 hPa incl. battery and calibration protocol

Part no.

0560 5211

Precision pressure probe, 100 Pa, in robust metal housing with impact protection, incl. magnet for fast attachment, to measure differential pressure and flow		Differential pressure probe	0 to +100 Pa	±(0.3 Pa ±0.5% of mv)	50 hPa	100 hPa	up to 20 Pa	0638 1347
speeds (in combination with Pitot tube)	Plug-in head, connection ca 0143 or 0430 0145 require							
Pressure probe, 10 hPa, in robust metal housing with impact protection incl. magnet for fast attachment, to measure differential pressure and flow speeds (in combination with Pitot tube)	8	Differential pressure probe	0 to +10 hPa	±0.03 hPa	50 hPa	1000 hPa	to 0,4 hPa	0638 1447
	Plug-in head, connection ca 0143 or 0430 0145 require							
Pressure probe, 100 hPa, in robust metal housing with impact protection, incl. magnet for fast attachment, to measure differential pressure and flow speeds (in combination with Pitot tube)		Differential pressure probe	0 to +100 hPa	±0.5% of mv (+20 to +100 hPa) ±0.1 hPa (0 to +20 hPa)	300 hPa	1000 hPa	to 4 hPa	0638 1547
	Plug-in head, connection ca or 0430 0145 required	ble 0430 0143		TH M				
Pressure probe, 2000 hPa, measures absolute pressure, in robust metal housing with impact protection, incl. quick-closing coupling (M8 x 0.5), magnet for fast		Absolute pressure probe	0 to +2000 hPa	±5 hPa (0 to +2000 hPa	a)4000 hPa	=	=	0638 1847
attachment	Plug-in head, connection ca 0143 or 0430 0145 require							

Probe type Meas. range Accuracy

Prandtl's Pitot tubes	Illustration			Meas. range	Part no.
Pitot tube, 300 mm long, stainless steel, for measuring flow velocity		300 mm	Ø 4 mm	Oper. temp. 0 to +600 °C	0635 2245
Pitot tube, 350 mm long, Ø 7 mm, stainless steel, measures flow speed		350 mm	Ø 7 mm	Oper. temp. 0 to +600 °C	0635 2145
Pitot tube, 500 mm long, Ø 7 mm, stainless steel, measures flow speed		500 mm	Ø 7 mm	Oper. temp. 0 to +600 °C	0635 2045
Pitot tube, 1000 mm long, stainless steel, measures flow speed		1000 mm	Ø 7 mm	Oper.temp. 0 to +600 °C	0635 2345

Straight Pitot tubes	Illustration		Probe type	Meas. range	Part no.
Pitot tube, stainless steel, 360 mm long, for measuring flow velocity incl.temperature, for pressure probes 0638 1347/1447/1547	360 mm	Ø 8 mm	Type K (NiCr-Ni)	-40 to +600 °C	0635 2040
Pitot tube, stainless steel, 500 mm long, for measuring flow velocity incl. temperature, for pressure probes 0638 1347/1447/1547	500 mm	Ø 8 mm	Type K (NiCr-Ni)	-40 to +600 °C	0635 2140
Pitot tube, stainless steel, 1000 mm long, for measuring flow velocity incl. temperature, for pressure probes 0638 1347/1447/1547	1000 mm	Ø 8 mm	Type K (NiCr-Ni)	-40 to +600 °C	0635 2240



testo 521-1 / testo 521-2 Additional probes, accessories and technical data

Probes	Illustration	Meas. range	Accuracy	t99	Part no.	
Pipe wrap probe for pipes up to 2" in diameter		-60 to +130 °C	Class 2*	5 s	0600 4593	
	Fixed cable					
Super quick-action immersion/penetration probe for measurements in liquids	150 mm =	0 1.5 mm -200 to +600 °C	Class 1*	1 s	0604 0493	
	Plug-in head. connection cable 0430 0143 or 0430 0145 required					
Highly accurate air probe for air and gas	150 mm	-40 to +130 °C	To UNI curve	60 s	0610 9714	
temperature measurements with bare,	-00	0.0				
mechanically protected sensor	Fixed cable	Ø 9 mm				

^{*} According to standard EN 60584-2, the accuracy of Classes 1 / 2 refer to -40 to +1000/+1200 °C.

Accessories		Part no.
Transport and Protection		
TopSafe (protection case) incl. carrier strap, bench stand and magnet. Protect	s instrument from dust, in	0516 0446 npact, scratches
Transport case for measuring instrument, probes, Prandtl Pitot tube	e, accessories	0516 0527
System case For measuring instrument, probes, straight or Prand	Itl Pitot tube, accessories	0516 0526
Additional Accessories and Spare Part	S	
9V rech. battery for instrument instead of battery		0515 0025
Desk-top power supply with international connection	n options	0554 1143
Cable, 1.5 m long, connects probe with plug-in hear PUR coating material	d to meas. instrument	0430 0143
Cable, 5 m long, connects probe with plug-in head to PUR coating material	to measuring instrument	0430 0145
Connection hose, silicone, 5m long max. load 700 hPa (mbar)		0554 0440
Printer and Accessories		
Testo fast printer with wireless infrared interface, 1 and 4 AA batteries	roll thermal paper	0554 0549
Spare thermal paper for printer (6 rolls), permanent measurement data documentation legible for up to		0554 0568
Software and Accessories		
ComSoft 3 - Professional with data management incl. database, analysis and graphics function, data	analysis, trend curve	0554 0830
RS232 cable connects instrument to PC (1.8 m) for data transfer		0409 0178
Ethernet adapter, RS232 - Ethernet incl. software dr facilitates data communication in network	river, mains unit	0554 1711
Calibration Certificates		
DAkkS calibration certificate/pressure* diff. and pos. pressure; 11 measuring points distribu	uted over the instr. meas.	0520 0215 range
DAkkS calibration certificate/pressure* diff. and pos. pressure; 6 meas. points distributed o	ver meas. range (>0.6% (0520 0225 of fsv)
DAkkS calibration certificate/pressure* absolute pressure; 11 measuring points distributed	over meas. range	0520 0212
ISO calibration certificate/pressure differential pressure, accuracy 0.1 to 0.6 (% of fsv)		0520 0025
ISO calibration certificate/pressure differential pressure; 5 points distributed over meas	. range	0520 0005
ISO calibration certificate/absolute pressure, 5 measurement points disabsolute pressure, accuracy 0.1 to 0.6 (% of fsv) $$	stributed over meas, range	0520 0125

ŀ	Accura	te m	easur	emen	ts t	rom	1	m/	S

*Successor organization of the DKD

You will achieve accurate measurement results in the range from 5 to 100 m/s using an internal pressure sensor with an accuracy of 0.1 % of fsv:

Accuracy at 5 m/s: 0.32 m/s
Accuracy at 20 m/s: 0.09 m/s
Accuracy at 50 m/s: 0.05 m/s

High accuracy levels are achieved in the velocity range from 1 to 12 m/s when you use the 100 Pa probe which is connected externally. Dependencies on position are completely eliminated thanks to double diaphragm engineering. Changes in position do not influence the measurement result:

Accuracy at 1 m/s: 0.09 m/s
Accuracy at 5-8 m/s: 0.03 m/s

Technical data		
	testo 521-1	
Probe type	Piezoresistive pressure sensor (built in to the instrument)	
Meas. range	0 100 hPa	
Overload	300 hPa	
Static pressure	2000 hPa	
Accuracy ±1 digit	±0.2 % of fsv	
Resolution	0.01 hPa	

	testo 521-2		
Probe type	Piezoresistive pressure sensor (built in to the instrument)	Pitot tube measurement	
Meas. range	0 to 100 hPa	5 to 100 m/s	
Overload	300 hPa		
Static pressure	2000 hPa		
Accuracy ±1 digit	±0.1 % of fsv	0.05 m/s at 65 m/s	
Resolution	0.01 hPa		

Common data				
Probe type	Plezoresistive pressure sensor for external pressure probes	NTC	Type K (NiCr-Ni)	
Meas. range	0 to 2000 hPa	-40 to +150 °C	-200 to +1370 °C	
Accuracy ±1 digit	±0.1 % of mv	±0.2 °C (-10 to +50 °C) ±0.4 °C (remaining range)	±0.4 °C (-100 to +200 °C) ±1 °C (remaining range)	
Resolution	0.1 Pa (0638 1347) 0.001 hPa (0638 1447) 0.01 hPa (0638 1547) 0.1 hPa (0638 1847)	0.1 °C	0.1 °C	

Oper. temp. (compensated)	0 to +50 °C
Storage temp.	-20 to +70 °C
Display	LCD display with symbol, 7 segment display and point matrix LCD, 2 lines
Battery type	9 V (6LR61)
Dimensions	219 x 68 x 50 mm
Weight	300 g
PC	RS232 interface
Memory	25,000

Power supply	Battery/Rechargeable battery/Wains unit 12V
Battery life	Continuous operation w/ internal pressure sensor: 30 h With rech. battery: 10 h With carbon battery: 18 h
Other features	Mains connection and battery recharging in instrument Automatic recognition of all connected probes
Material/Housing	ABS
Warranty	2 years

Pitot tube measurement

Straight Pitot tubes or classical Prandth's Pitot tubes can be used, depending on the application. Pitot tubes are available in different lengths and diameters depending on duct diameters and duct openings.



Straight Pitot tubes

- Built-in temperature measurement
- Higher accuracy on account of Pitot tube factor 0.67
- Application range from -40 to +600 °C



- Higher velocity range in pressure measurement range used
- Application range from 0 to +600 °C

testo 512 shows pressure and flow velocity simultaneously in an easy-to-read, large, backlit display. Measurement data is printed on site with date and time as well as minimum and maximum values. testo 512 has two switchable units for flow: m/s and fpm. Eight units can be set for pressure: kPa, hPa, Pa, mmH2O, mmHg, psi, inch H2O, inch Hg.

Adjustable damping for sliding mean calculation, density compensation is built-in. The displayed actual value can be frozen in the display by pressing the HOLD button. The measured minimum and maximum value can be displayed and stored in the meter.

TopSafe protects the measuring instrument in the field from impact, dirt and splash water.

Pressure and flow velocity measuring instrument

- 8 units for pressure: kPa, hPa, Pa, mm H₂O, mmHg, psi, inch H₂O, inch Hg
- 2 units for flow: m/s, fpm
- Built-in density compensation
- Display light
- Hold/Max/Min function
- Readings printout with date/time and min./max. values



 Simultaneous display of flow and pressure value

0 to 2 hPa/mbar

testo 512 differential pressure meter, 0 to 2 hPa, incl. battery and calibration protocol

Part no.

0560 5126

2 0 to 20 hPa/mbar testo 512 differential pressure meter, 0 to 20 hPa, incl. battery and calibration protocol

Part no.

0560 5127

0 to 200 hPa/mbar testo 512 differential pressure meter, 0 to 200 hPa, incl. battery and calibration protocol

Part no.

0560 5128

4 0 to 2000 hPa/mbar w/o flow velocity and Pascal measurement

testo 512 differential pressure meter, 0 to 2000 hPa, incl. battery and calibration protocol

Part no.

0560 5129

Technical data				
	1	2	3	4
Meas. range	0 to +2 hPa +2 to +17.5 m/s 395 to 3445 fpm	0 to +20 hPa +5 to +55 m/s 985 to 10830 fpm	0 to +200 hPa +10 to +100 m/s 1970 to 19690 fpm	0 to +2000 hPa
Resolution	0.001 hPa 0.1 m/s 0.1 fpm	0.01 hPa 0.1 m/s 0.1 fpm	0.1 hPa 0.1 m/s 0.1 fpm	1 hPa
Overload	±10 hPa	±200 hPa	±2000 hPa	±4000 hPa

Common data			
Accuracy	0.5% of fsv ± 1 digit	Auto Off	10 min
Measuring medium	All non-corrosive gases	Battery type	9V block battery, 6F22
		Battery life	120 h
Display	LCD, 2 lines	Dimensions	202 x 57 x 42 mm
Oper. temp.	0 to +60 °C	Weight	300 g
Storage temp.	-10 to +70 °C	Warranty	2 years

Accessories	Part no.
Accessories for measuring instrument	
9V rech. battery for instrument instead of battery	0515 0025
Recharger for 9V rechargeable battery for external recharging of 0515 0025 battery	0554 0025
Printer and accessories	
Testo fast printer with wireless infrared interface, 1 roll thermal paper and 4 $$ AA batteries $$	0554 0549
Spare thermal paper for printer (6 rolls), permanent ink measurement data documentation legible for up to 10 years	0554 0568
Transport and Protection	
TopSafe, protects from impact and dirt	0516 0221
Case for measuring instrument and probes	0516 0210
Transport case for meas, instr. and probes (405 x 170 x 85 mm)	0516 0201

Accessories	Part no.					
Additional accessories and spare parts						
Pitot tube, 350 mm long, Ø 7 mm, stainless steel, measures flow speed	0635 2145					
Pitot tube, 500 mm long, Ø 7 mm, stainless steel, measures flow speed	0635 2045					
Pitot tube, 1000 mm long, stainless steel, measures flow speed	0635 2345					
Connection hose, silicone, 5m long max. load 700 hPa (mbar)	0554 0440					
Calibration certificates						
DAkkS calibration certificate/pressure* diff. and pos. pressure; 11 measuring points distributed over the instr. mea	0520 0215 s. range					
ISO calibration certificate/pressure, differential pressure, accuracy 0.1 to 0.6 (% of fsv)	0520 0025					
*Successor organization of the DKD						



Mini wind tunnel

You can draw up your own ISO certificates using the wind tunnel and a certified Testo measuring instrument. All of Testo's velocity probes can be checked and calibrated using the mini wind tunnel (except Ø 100 mm vane probes).

Draw up your own ISO calibration certificates! The Testo mini wind tunnel can be used for regular checks on velocity probes and measuring instruments in your company.

- 3 speed levels can be set: 2.5/5/10 m/s
- The readings are traceable to the PTB standard if Testo's DAkkS certified testo 400 reference instrument is
- used

Accuracy of wind tunnel: ±1 % of reading (at least 0.1 m/s) plus calibration uncertainty of the respective reference instrument's certificate



Recommended set

Testo mini wind tunnel, affordable set for beginners

- Mini wind tunnel incl. power connection cable (Part no. 0554 0450)
- testo 435-2, multi-functional measuring instrument for A/C, ventilation and Indoor Air Quality with readings memory, PC software and USB data transmission cable, incl. battery and calibration protocol (Part no. 0563 4352)
- Vane meas. probe, 16 mm diameter, with telescopic handle max. 890 mm, e.g. for meas. in ducts (Part no. 0635 9535)
- DAkkS calibration certificate/velocity* (Part no. 0520 0254)

You already have a Testo measuring instrument with velocity probe and calibration certificate and you want to calibrate more probes of the same type using the wind tunnel. Mini wind tunnel incl. power connection cable

Part no.

0554 0450

Technical data

Lenath: 610 mm Ø meas. tunnel: approx. 100 mm (inside) Velocities: 2.5/5/10 m/s, can be switched Range of application: +10 to +40 °C Probe holder: For all of Testo's velocity probes except vane probes with Ø 100

Motor: Direct current fan Power supply: 230 V/50 Hz or 110 V can be switched, built-in IEC socket Warranty: 2 years

Testo mini wind tunnel with reference measuring system

- Mini wind tunnel incl. power connection cable (Part no. 0554 0450)
- testo 400, multi-function measuring instrument, incl. store for up to 500,000 readings, VAC module (volume flow measurement with error calculation), battery, Li cell and calibration protocol (Part no. 0563 4001)
- Vane/temperature probe, Ø 16 mm, attachable to 0430 3545 handle or 0430 0941 telescopic handle(Part no. 0635 9540)
- Cable, 1.5 m long, for connecting vane probes with plug-in head to the measuring instrument (Part
- DAkkS calibration certificate/velocity* (Part no. 0520 0254)

*Successor organization of the DKD

Testo fast printer

Universal infrared printer for differential pressure measuring instrument testo 512

The universal printer with IRDA and infrared interface saves you time since it stores the print data prior to printing. Data transfer is completed within 2 seconds. The instrument is then immediately ready for operation.

The readings are saved black on white with date and time.

Testo fast printer with wireless infrared interface, 1 roll thermal paper and 4 AA batteries

Part no.

0554 0549

- System compatibility with other Testo measuring instruments (also downward compatibility)
- Fast data transfer, the measuring instrument is ready for use again within 2 sec.
- Fast print function thanks to newest

Energy-saving Auto-off/Wake-up

function

Testo design with integrated magnetic

plate

Robust housing (adapted to testo

327)

Mains operation possible (same

mains unit as for testo 327/330)



	recnnicai data				
Printer type	infrared-controlled	C	Oper. temp.	0 to +50 °C	
	thermal printer,	S	Storage temp.	-40 to +60 °C	
	adjustable contrast, graphic-capable	P	Power supply	4 AA batteries 1.5 V (or rechargeables) Mains unit GV/1.2A	
	Reception radius	max. 2 m	٧	Veight	430 g
	Dimensions	147 x 77 x 47 mm			


Accessories	Part no.
Spare thermal paper for printer (6 rolls)	0554 0569
Spare thermal paper for printer (6 rolls), permaner documentation legible for up to 10 years	nt ink, measurement data 0554 0568
External fast charger for 1-4 AA rech. batteries, in with individual cell charging and charge control discharging, integrated discharge function, with built-	splay, incl. impulse trickle

plug, 100-240 V, 300 mA, 50/60 Hz

structure - measure - print on-site

Structuring measurement data:

- Readings can be saved at individual locations - with guarantee of refinding.
- The "tree structure" folders, sub-folders and measurement protocols guarantees an uncomplicated overview.
- Practical additional information such as measurement information or required value input can be saved with the location.
- The locations can be selected via barcode labels using the pen.
- It is easy to draw an effective tour plan using the locations list.

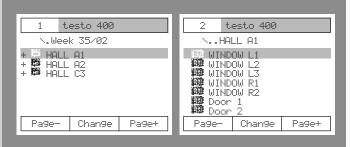


Long-term control made easy:

User-friendly data logging, not only for spot checks


- The beginning of the measurement can be...
 - determined manually each time.
 - activated if a user defined limit value is exceeded.
 - set according to date/time.
- The measurement is completed when...
 - the predefined number of readings is reached.
 - date/time is reached.
 - the memory is full.
 - ended manually.
- · Non-stop measurement via wrap-around memory...
 - deletes the oldest respective value.
 - is deactivated manually.





Documentation on-site:

- The individual measurement protocol can be either saved or deleted following analysis.
- The fast printer immediately supplies the documentation required.
- The attachable comfort printer also offers graphical analysis options.
- Thermal paper for long-term legible measurement data documentation of up to 10 years.

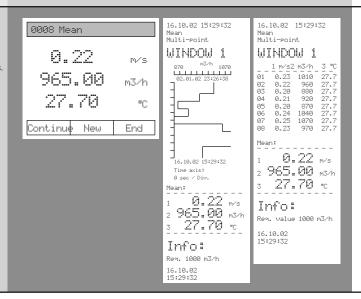




prepare - analyse - file - document


Easy reading management:

- Preparation of the measurement:
- The measurement program is determined and loaded into instrument
- Tour plan is drawn up based on locations and is loaded into instrument.
- The measuring instrument is downloaded once measuring is complete:
 - The saved protocols are conveniently filed via the software using "Drag & Drop" or are analysed in Data.
- The readings are determined using the measuring instrument and can also be displayed online using the software.

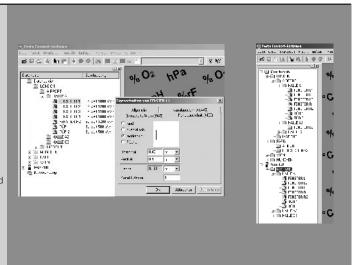


Comprehensive analysis, easy filing:

- · Analysis:
 - with calculation functions
 - with crosshairs
 - with mean calculation
 - with calculation of standard deviation
 - taking all conventional refrigerants into consideration (refrigeration module, optional)
- Display:
- as table or as graphic
- as digit field or as histogram
- with analog display
- Measurement channels can be activated or deactivated at the touch of a button
- Documenting:
- Data is transferred to Excel table using "Copy and Paste".

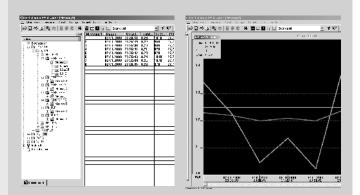

Individual configuration options:

- Your company logo can be included on the printouts.
- Functions can be selected from the function list and the finished profile can be saved.
- The online interface is available for LabVIEW software.
- Menu can be individually tailored to your needs.

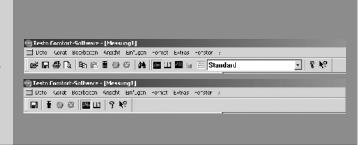

ComSoft 3 - Professional for:

- Monitoring measuring instrument testo 445
- Reference measuring instrument testo 400

ComSoft 3 - Professional with data management				
function, data analysis, tre	function, data analysis, trend curve			
Part no.				
0554 0830				

Accessories Part no.
RS232 cable 0409 0178
connects instrument to PC (1.8 m) for data transfer

Ethernet adapter

The Ethernet adapter enables the following:

- On-site measurements, e.g. in production, warehouses, Incoming Goods
- Measuring instrument remains on site, transport not necessary
- Data inspection from office or administration
- Centralised filing of measurement data

Ethernet offers:

- · Fast transmission of readings
- Use of an existing network without additional cabling
- Long transmission distances
- Identification of measuring instruments in system network

Ethernet adapter, RS232 - Ethernet incl. software driver, mains unit facilitates data communication in network (not for use in Ex-zone)

Part no.

0554 1711

Access Ethernet with Testo measuring instruments

Multi-point checks on site

Testo's portable measuring instruments are used in production or in Incoming Goods to take spot checks on site. Using an Ethernet adapter, measurement data can be transmitted immediately to a central office which enables fast reaction times, if further actions are required.



Accessories	Pai	t no.
System accessories: testo 400, testo	445	
ComSoft 3 - Professional with data management, and graphics function, data analysis, trend curve	incl. database, analysis 055	4 0830
RS232 cable, connects instrument to PC (1.8 m) to	for data transfer 040	9 0178

Technical data				
Dimensions	45 x 48 x 14 mm		Management and software configuration	Internet browser e.g. from Netscape or
Oper. temp.	+0 to +70 °C			
Software	Microsoft Windows 2000 / NT 4.0 / ME / 98 / 95			Microsoft Telnet
Power supply	Mains unit, 5 Volt app. 230 mA		Interface	Serial interface on computer board with
Humidity class	F to DIN 40040			terminal program
EMC	Radio interference and interference resistance			Provision of a local virtual COM port (Windows
Interface	25 pin RS 232 connection with adapter 25/9pin			systems)
Logs	TCP/IP, LPR, Telnet, SNMP, DHCP DDNS, ARP, BOOTP, ICMP			



The testo 445 VAC instrument measures temperature, relative humidity, dew point, absolute humidity, degree of humidity, enthalpy, all types of air velocity (in ducts, duct openings or extractors), volume flow, pressure and indoor air quality.

Data can be saved according to location and then analysed on PC or printed on the Testo fast printer on site.

testo 445, VAC measuring instrument, incl. TopSafe, battery and calibration protocol

Part no.

0563 4450

Service instrument for ventilation/air conditioning systems

- Automatic mean calculation and volume flow measurement
- Automatic allocation of duct crosssection to location (max. 99 locations)
- Internal data logger (3,000 readings)
- Simultaneous measurement of up to 6 parameters





Practical accessories and technical data

	Part no.
Transport and Protection	0540 0445
ransport case (plastic) for measuring instrument, probes and accessories arger version, for safe and clear storage	0516 0445
ystem case (plastic) for measuring instrument, probes and accessories robes in lid make it easy to find parts in case (540 x 440 x 130 mm)	0516 0400
ystem case (aluminium) for measuring instrument, probes and accessories robes in lid make it easy to find parts in case	0516 0410
Additional Accessories and Spare Parts	
V rech. battery for instrument stead of battery	0515 0025
esk-top power supply with international connection options	0554 1143
able, 1.5 m long, connects probe with plug-in head to meas. instrument UR coating material	0430 0143
able, 5 m long, connects probe with plug-in head to measuring instrument UR coating material	0430 0145
xtension cable, 5 m long, between plug-in head cable and instrument UR coating material	0409 0063
Printer and Accessories	
esto fast printer with wireless infrared interface, 1 roll thermal paper and 4 A batteries	0554 0549
ast testo 575 printer, incl. 1 roll of thermal paper and batteries ifrared thermal line printer with graphics function	0554 1775
xternal fast charger for 1-4 AA rech. batteries, incl. 4 Ni-MH rech. batteries ith individual cell charging and charge control display, incl. impulse trickle harging, integrated discharge function, with built-in international mains lug, 100-240 V, 300 mA, 50/60 Hz	5 0554 0610
pare thermal paper for printer (6 rolls)	0554 0569
pare thermal paper for printer (6 rolls), permanent ink neasurement data documentation legible for up to 10 years	0554 0568
abel thermal paper (Testo patent) for testo 575 printer (6 rolls), can be pplied directly	0554 0561
Software and Accessories	
omSoft 3 - Professional with data management ccl. database, analysis and graphics function, data analysis, trend curve	0554 0830
S232 cable onnects instrument to PC (1.8 m) for data transfer	0409 0178
thernet adapter, RS232 - Ethernet incl. software driver, mains unit acilitates data communication in network	0554 1711
Calibration Certificates	
60 calibration certificate velocity of wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s	0520 0004
SO calibration certificate/Velocity ot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s	0520 0034
AkkS calibration certificate/velocity* ot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s	0520 0244
	0520 0204
AkkS calibration certificate/velocity* ot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m	

Technical data			
Probe type	Type K (NiCr-Ni)	Type J (Fe-CuNi)	NTC
Meas. range	-200 to +1370 °C	-200 to +1000 °C	-50 to +150 °C
Accuracy ±1 digit	±0.5% of mv (-200 to 60 °C) ±0.5% of mv (+60 to +1370 °C) ±0.3 °C (-60 to +60 °C)	±0.5% of mv (-200 to 60 °C) ±0.5% of mv (+60 to +1000 °C) ±0.3 °C (-60 to +60 °C)	
Resolution	0.1 °C (-200 to +1370 °C)	0.1 °C (-200 to +1000 °C)	0.1 °C (-50 to +150 °C)

Probe type	Testo humid. sensor, cap.	Vane	Thermal
Meas. range	0 to +100 %RH	0 to +60 m/s	0 to +20 m/s
Accuracy ±1 digit	See probe data	See probe data	See probe data
Resolution	0.1 %RH (0 to +100 %RH)	0.01 m/s (0 to +60 m/s)	0.01 m/s (0 to +10 m/s) 0.1 m/s (+10.1 to +20 m/s)

Probe type	Pressure	CO2 probe	CO2 probe
Meas. range	See pressure probes	0 to +1 Vol. % CO ₂	0 to +10000 ppm CO ₂
Accuracy ±1 digit	±0.1% of mv	See probe data	$\begin{array}{l} \pm (100 \; \mathrm{ppm} \; \mathrm{CO_2} \pm 3\% \; \mathrm{of} \; \mathrm{mv}) \\ (+5000 \; \mathrm{to} \; +10000 \; \mathrm{ppm} \; \mathrm{CO_2}) \\ \pm (500 \; \mathrm{ppm} \; \mathrm{CO_2} \pm 2\% \; \mathrm{of} \; \mathrm{mv}) \\ (0 \; \mathrm{to} \; +5000 \; \mathrm{ppm} \; \mathrm{CO_2}) \end{array}$
Resolution	0.001 hPa (Sonde 0638 1345) 0.001 hPa (Sonde 0638 1445) 0.01 hPa (Sonde 0638 1545) 1 hPa (Sonde 0638 1645)	0 Vol. % CO ₂ (0 to +1 Vol. % CO ₂)	1 ppm CO ₂ (0 to +10000 ppm CO ₂)

Probe type	CO probe	
Meas. range	0 to +500 ppm CO	
Accuracy ±1 digit	±5% of mv (+100 to +500 ppm CO) ±5 ppm CO (0 to +100 ppm CO)	
Resolution	1 ppm CO (0 to +500 ppm CO)	

0 to +50 °C
-20 to +70 °C
LCD, 4 lines
9V block battery
45 h
RS232 interface
255 g
ABS
2 years
3000
215 x 68 x 47 mm

Battery life: 6-45 h (depending on probe) Mains conn. and batt. rech. in instr. Calculated humidity parameters: td, g/m3, g/kg pressure-compensated, J/g Calculated volume flow: m3/h (e.g. 0 to 99999 m3/h), m3/min, m3/s, l/s, cfm
Calculated velocity values (density-compensated): 0 to 100 m/s; 0 to 99999 m3/h Humidity measurement: Measuring range -50 to 180°C; See Probes for accuracy Accuracy of Type K, J: Additional error via operation temperature 0.2 °C (adjustment point)



Probes	Illustration	Probe type	Meas. range	Accuracy	Part no.
Vane probe, Ø 12 mm, can be attached to handle 0430 3545 or telescopic handle 0430 0941	180 mm Ø 12 mm	Vane	+0.6 to +20 m/s Oper. temp. -30 to +140 °C	$\pm (0.2 \text{ m/s} \pm 1\% \text{ of mv})$ (+0.6 to +20 m/s)	0635 9443
Vane/temperature probe, Ø 16 mm, attachable to 0430 3545 handle or 0430 0941 telescopic handle	180 mm Ø 16 mm	Vane Type K (NiCr-Ni)	+0.4 to +60 m/s -30 to +140 °C	±(0.2 m/s +1% of mv) (+0.4 to +40 m/s) ±(0.2 m/s +2% of mv) (+40.1 to +50 m/s)	0635 9540
Vane/temperature probe, Ø 25 mm, can be attached to 0430 3545 handle or 0430 0941 telescopic handle	180 mm 0 25 mm	Vane Type K (NiCr-Ni)	+0.4 to +40 m/s -30 to +140 °C	±(0.2 m/s ±1% of mv) (+0.4 to +40 m/s)	0635 9640
Bendable vane probe (can be bent by 90°), Ø 60 mm, attachable to handle 0430 3545 or telescopic handle 0430 0941, for meas. on ventilation outlets	Ø 60 mm	Vane	+0.25 to +20 m/s Oper. temp. 0 to +60 °C	±(0.1 m/s ±1.5% of mv) (+0.25 to +20 m/s)	0635 9440
Bendable vane probe (can be bent by 90°), Ø 100 mm, attachable to handle 0430 3545 or telescopic handle 0430 0941, for measurements on ventilation outlets	Ø 100 mm	Vane	+0.1 to +15 m/s Oper. temp. 0 to +60 °C	±(0.1 m/s ±1.5% of mv) (+0.1 to +15 m/s)	0635 9340
Affordable, robust hot bulb probe, Ø 3 mm, for measurements in the lower velocity range, with handle	150 mm Ø 4 mm Ø 3 mm	Hot bulb NTC	0 to +10 m/s -20 to +70 °C	±(0.03 m/s ±5% of mv) (0 to +10 m/s)	0635 1549
Robust hot bulb probe, Ø 3 mm, with handle and telescopic handle for measurements in the lower velocity range	850 mm Ø 3 mm	Hot bulb NTC	0 to +10 m/s -20 to +70 °C	±(0.03 m/s ±5% of mv) (0 to +10 m/s)	0635 1049
Quick-action hot wire probe, Ø 10 mm, with telescopic handle, for measurements in the lower velocity range with direction recognition	760 mm Ø 10 mm	Hot wire NTC	0 to +20 m/s -20 to +70 °C	±(0.03 m/s ±4% of mv) (0 to +20 m/s)	0635 1041
Vane probe, Ø 16 mm, with telescopic handle, Tmax +60°C	700 mm Ø 16 mm	Vane	+0.6 to +40 m/s	$\pm (0.2 \text{ m/s} \pm 1.5\% \text{ of mv}) (+0.6 \text{ to } +40 \text{ m/s})$	0628 0005
Vane probe, Ø 60 mm, with telescopic handle, for integrating velocity measurement	0 60 mm	Vane	+0.25 to +20 m/s	±(0.1 m/s ±1.5% of mv) (+0.25 to +20 m/s)	0635 9449
High temperature vane probe, Ø 25 mm, with handle for continuous measurements up to +350°C	560 mm 0 25 mm	Vane Type K (NiCr-Ni)	+0.6 to +20 m/s -40 to +350 °C	±(0.3 m/s ±1% of fsv) (+0.6 to +20 m/s)	0635 6045
Precision pressure probe, 100 Pa, measures differential pressure and velocities (in combination with Pitot tube)	- HAMANA MARKET COMMITTEE	Differential pressure probe	0 to +100 Pa	±(0.3 Pa ±0.5% of mv) (0 to +100 Pa)	0638 1345
Pressure probe, 10 hPa, measures differential pressure and velocities (in combination with Pitot tube)	- Constant Constant	Differential pressure probe	0 to +10 hPa	±0.03 hPa (0 to +10 hPa	0638 1445



testo 445	Suitable probes at a g	lance			
Probes	Illustration	Probe type	Meas. range	Accuracy	Part no.
ressure probe, 100 hPa, measures differential ressure and velocities (in combination with Pitot ube)		Differential pressure probe	0 to +100 hPa	±0.5% of mv (+20 to +100 hPa) ±0.1 hPa (0 to +20 hPa)	0638 1545
Pressure probe, 2000 hPa, measures absolute ressure	- HOUSENS SANG	Absolute pressure probe	0 to +2000 hPa	±5 hPa (0 to +2000 hPa)	0638 1645
itot tube, 500 mm long, Ø 7 mm, stainless steel, leasures flow speed	500 mm	Ø 7 mm	Oper. temp. 0 to +600 °C		0635 2045
itot tube, 350 mm long, Ø 7 mm, stainless steel, leasures flow speed		Ø 7 mm	Oper. temp. 0 to +600 °C		0635 2145
itot tube, 300 mm long, stainless steel, for leasuring flow velocity	300 mm	Ø 4 mm	Oper. temp. 0 to +600 °C		0635 2245
Pitot tube, 1000 mm long, stainless steel, neasures flow speed	1000 mm	Ø 7 mm	Oper. temp. 0 to +600 °C		0635 2345
1-function probe for simultaneous measurement of emperature, humidity and velocity. With plug-in head, 1430 0143 connection cable required	270 mm	Hot bulb Testo humid. sensor, cap. NTC	0 to +10 m/s 0 to +100 %RH -20 to +70 °C	±(0.03 m/s ±5% of mv)(0 to 10 m/s) ±2 %RH (+2 to +98 %RH) ±0.4 °C (0 to +50 °C)	0635 1540
omfort level probe for measuring degree of turbulence, rith telescopic handle and stand. Fulfills EN 13779 aquirements	890 mm 0 90 mm	Hot wire NTC	0 to +5 m/s 0 to +50 °C	±0.5 °C (remaining range) ±(0.03 m/s ±4% of mv) (0 to +5 m/s) ±0.3 °C (0 to +50 °C)	0628 0009
02 probe measures indoor air quality and monitors the vorkplace. With plug-in head, connection cable 0430 1143 or 0430 0145 required		CO2 probe	0 +1 Vol. % CO ₂ 0 +10000 ppm CO ₂	±(50 ppm CO ₂ ±2% of mv)(0 +5000 ppm CO ₂) ±(100 ppm CO ₂ ±3% of mv)(+5001 to +10000 ppm CO ₂)	0 0632 1240
Ambient CO probe, for detecting CO in buildings and rooms			0 to +500 ppm C0	±5% of mv (+100.1 to +500 ppm CO) ±5 ppm CO (0 to +100 ppm CO)	0632 3331
More probes	Illustration	Meas. range Accuracy		t90	Part no.
tandard ambient air probe up to +70°C	Ø 12 mm Plug-in head. connection cable 0430 0143 or 0430 0145	0 to +100 %RH ±2 %RH (+2 to -20 to +70 °C %RH)	±0.4 °C (-10 to ±0.5 °C (remai		0636 9740
ouct humidity/temperature probe	180 mm	0 to +100 %RH ±2 %RH (+2 to -20 to +70 °C %RH)	±0.4 °C (-10 to ±0.5 °C (remai		0636 9715
hin humidity probe incl. 4 attachable protection caps for mbient air measurements, measurements in exhaust air ucts and equilibrium moisture measurements	250 mm 0 4 mm Plug-in head. connection cable 0430 0143 or 0430 0145	0 to +100 %RH ±2 %RH (+2 to -20 to +70 °C %RH)	±0.4 °C (-10 to ±0.5 °C (-20 to ±0.5 °C (+50.7	-10.1 °C)	0636 2130
lighly accurate reference humidity/temp. probe	0 21 m Plug-in head. connection cable 0430 0143 or 0430 0144	0 to +100 %RH ±1 %RH (+10 to %RH)* +2 %RH (remaining	±0.4 °C (remai		0636 9741
lexible humidity probe with mini module for neas. e.g. on material testing rigs, module cable ength 1500mm, probe tip 50x19x7mm	Plug-in head. connection cable 0430 0143 or 0430 0144	0 to +100 %RH	±0.4 °C (-10 to ±0.5 °C (remai		0628 0013
word probe for measuring humidity and emperature in stacked material	320 mm 18 mm x 5 mm Plug-in head. connection cable 0430 0143 or 0430 0145	0 to +100 %RH	±0.4 °C (-10 to ±0.5 °C (-20 to ±0.5 °C (+50.1	o -10.1 °Ć)	0636 0340
ligh humidity level probe w/ heated sensor element, no humidity on sensor	300 mm 0 12 mm Plug-in head. connection cable 0430 0143 or 0430 0145	0 to +100 %RH	±0.4 °C (-10 to ±0.5 °C (-20 to ±0.5 °C (+50.	o -10.1 °C)	0636 2142

Robust humidity probe e.g. for measuring equilibrium moisture or for measurements in exhaust ducts to +120°C

Robust high temperature/humidity probe up to +180°C

Flexible humidity probe (does not retain shape) for measurements in inaccessible places

Standard pressure dew point probe for measurements in compressed air systems

Precision pressure dew point probe for measurements in compressed air systems incl. cert. with test point -40°C tpd

300 mm	A.
Plug-in head. connection cable	e 0430 0143 or 0430 0145 re
300 mm	de.

Plug-in head. connection cable 0430 0143 or 0430 0145 required

0 to +100 %RH -60 to +50 °C tpd

0 to +100 %RH -20 to +180 °C

0 to +100 %RH -20 to +120 °C

0 to +100 %RH -20 to +180 °C

Ø 12 mm

300 mm

Ø 12 mm

Ø 12 mm

100 mm

Plug-in head. connection cable 0430 0143 or 0430 0145 required

Plug-in head. connection cable 0430 0143 or 0430 0145 required

±2 %RH (+2 to +98 %RH)

±2 %RH (+2 to +98 %RH)

 $\begin{array}{l} \pm 0.9~^{\circ}\text{C tpd}~(+0.1~\text{to}~+50~^{\circ}\text{C tpd}) \\ \pm 1~^{\circ}\text{C tpd}~(-4.9~\text{to}~0~^{\circ}\text{C tpd}) \\ \pm 2~^{\circ}\text{C tpd}~(-9.9~\text{to}~-5~^{\circ}\text{C tpd}) \\ \pm 3~^{\circ}\text{C tpd}~(-19.9~\text{to}~-10~^{\circ}\text{C tpd}) \\ \pm 4~^{\circ}\text{C tpd}~(-30~\text{to}~-20~^{\circ}\text{C tpd}) \end{array}$ ±0.8 °C tpd (-4.9 to +50 °C tpd) ±1 °C tpd (-9.9 to -5 °C tpd) ±2 °C tpd (-19.9 to -10 °C tpd) ±3 °C tpd (-29.9 to -20 °C tpd) ±4 °C tpd (-40 to -30 °C tpd)

±0.4 °C (-10 to +50 °C) ±0.5 °C (remaining range)

 $\begin{array}{ccc} \pm 2 \text{ %RH (+2 to +98} & \pm 0.4 \text{ °C (+0.1 to +50 °C)} \\ \text{ %RH)} & \pm 0.5 \text{ °C (remaining range)} \end{array}$

±0.4 °C (+0.1 to +50 °C) ±0.5 °C (-20 to 0 °C) ±0.5 °C (+50.1 to +180 °C) 0636 9840 300 300 0636 9841

30 s

30 s

0636 2140

0628 0021

0628 0022

 $^{^{\}star}$ in the temperature range from +15°C to +30°C



Plug-in head. connection cable 0430 0143 or 0430 0145 required 0 to +100 %RH -30 to +50 °C tpd



Suitable probes at a glance

Probes	Illustration	Meas. range	Accuracy	t99	Part no.
Quick-action surface probe with sprung thermocouple strip, measuring range short-term to +500 °C	150 mm	-200 to +300 °C	Class 2*	3 s	0604 0194
0 +500 C	Plug-in head. connection cable 0430 0143 or 0430 0145 requ	ired			
Super quick-action immersion/penetration probe for measurements in liquids	150 mm 0 1.5 mm Plug-in head. connection cable 0430 0143 or 0430 0145 requ	-200 to +600 °C	Class 1*	1 s	0604 0493
Super quick-action immersion/penetration probe for measurements in gases and liquids with a ow-mass tip	150 mm 0 1.4 mm Plug-in head. connection cable 0430 0143 or 0430 0145 requ	20 mm -200 to +600 °C 0 0.5 mm ired	Class 1*	1 s	0604 9794
Pipe wrap probe for pipes up to 2" in diameter	Fixed cable	-60 to +130 °C	Class 2*	5 s	0600 4593
Spare meas. head for pipe wrap probe, TC Type K	35 mm 15 mm	-60 to +130 °C	Class 2*	5 s	0602 0092
Globe thermometer to measure radiant heat	Ø 150 mm	accuracy corresponds to 0 to +120 °C SO 7243, ISO 7726, DIN N 27726, DIN 33403 squirements	±0.5 °C (0 to +49.9 °C) ±1 °C (+50 to +120 °C)		0554 0670

 $^{^{\}star}$ According to standard EN 60584-2, the accuracy of Classes 1 / 2 refer to -40 to +1000/+1200 °C.

See testo 400 for more probes

Accessories for velocity probes, pressure probes	Part no.
Professional telescopic handle for plug-in vane probes, max. 1 m long	0430 0941
Extension for telescopic handle, 2 m long please also order the 0409 0063 extension cable	0430 0942
Handle for plug-in vane probes	0430 3545
Extension cable, 5 m long, between plug-in head cable and instrument PUR coating material $$	0409 0063
Connection hose, silicone, 5m long max. load 700 hPa (mbar)	0554 0440
Cover plugs for test holes (50 off)	0554 4001

Accessories for temperature probes	Part no.
Silicone heat paste (14g), Tmax = +260°C improves heat transfer in surface probes	0554 0004
Cable, 1.5 m long, connects probe with plug-in head to meas. instrument PUR coating material	0430 0143
Cable, 5 m long, connects probe with plug-in head to measuring instrumen PUR coating material	t 0430 0145
Extension cable, 5 m long, between plug-in head cable and instrument PUR coating material $$	0409 0063
Telescopic handle, max. 1 m, for probe with plug-in head cable: 2.5 m long, PUR coating material	0430 0144

Accessories: Humidity, 3-function probe	Part no.
Cable, 1.5 m long, connects probe with plug-in head to meas. instrument PUR coating material	0430 0143
Cable, 5 m long, connects probe with plug-in head to measuring instrument PUR coating material	0430 0145
Extension cable, 5 m long, between plug-in head cable and instrument PUR coating material	0409 0063
Telescopic handle, max. 1 m, for probe with plug-in head cable: 2.5 m long, PUR coating material	0430 0144
testo saline pots for control and humidity adjustment of humidity probes, 11.3 %RH and 75.3 %RH with adapter for humidity probe	0554 0660
Metal protection cage, Ø 12 mm for humidity probes for measurement in flow velocities of less than 10 m/s	0554 0755
Cap with wire mesh filter, Ø 12 mm	0554 0757
PTFE sintered filter, Ø 21 mm, for corrosive substances nigh humidity range (long-term measurements), high velocities	0554 0666
Sintered PTFE filter, Ø 12 mm, for corrosive media High humidity range (long-term measurements), high flow velocities.	0554 0756
Stainless steel sintered cap, Ø 21 mm, can be screwed onto humidity probe protection in case of high mechanical load and high velocities	0554 0640
Stainless steel sintered cap, Ø 12 mm, is screwed onto humidity probe for measurements at higher flow velocities or in contaminated air	0554 0647
PTFE cap, Ø 5 mm, attachable, PTFE material, (5 off) PTFE Dust protection, high humidity measurements, high flow speeds for humidity orobe 0636 2130	0554 1031
PTFE sintered filter, Ø 12 mm, for corrosive substances nigh humidity range (non-stop measurements), high flow speeds	0554 0758

Caps for humidity probes, see page 32

Precision reference class measuring instruments have everything the professional user needs to complete complicated measurement tasks efficiently, accurately and conveniently.

testo 400 includes the parameters temperature, CO2, rpm, current, voltage, relative humidity, pressure, velocity and volume flow.

Intelligent electronics ensure the latest technology is used thanks to software updates. The measuring instrument can always keep up with the measurement tasks at hand thanks to upgrades.

Upgradable and teachable, highly reliable and of the highest quality they are the properties which guarantee that the customer is equipped for the future.

Useful instument functions:

- System accuracy up to 0.05 °C and up to a resolution of 0.001 °C
- All functions of testo 650 and testo 950
- Input of cross-sections for volume flow calculation
- Absolute pressure compensation in thermal probes
- Density calculation for velocity measurement with reference to temperature, humidity and absolute pressure
- Turbulence degree measurement to EN 13779
- Assessment of volume flow measurements with calculation of total uncertainty of measurement in accordance with EN 12599 with VAC module

The reference measuring instrument for A/C and ventilation systems

 VAC module for evaluating the measurement directly on site with integrated inaccuracy calculation

Clear graphics display

3 user defined function buttons

Save up to max. 500,000 readings) or print at the touch of a button

Mains connection/quick battery

Attachable printer (optional)


 Prints readings on site in a matter of seconds

Data communication via PC

 User friendly operation with cursor via menu structure

 Integrated reading memory for up to 500,000 readings

Possibility of remote connection via



Attachable printer prints readings on site in seconds

Clear graphics display


Data communication by PC

3 user-defined function buttons


Saves or prints at the touch of a button

Easy operation with cursor

Power connection/quick battery recharge 2 user defined probe sockets



Assessment of measurement directly on location with integrated uncertainty calculation



The coordinates required for the grid measurement are shown in the instrument display. The depth information on the vane telescopic handle makes the task that much easier in practice.

testo 400, multi-function measuring instrument, incl. store for up to 500,000 readings, VAC module (volume flow measurement with error calculation), battery, Li cell and calibration protocol

Can be used for:

- Velocity, volume flow
- · Humidity, pressure
- Temperature
- CO2, rpm and current/voltage

Part no.

0563 4001



Additional recommended sets

Recommended set

For fast measurements on VAC systems

- testo 400, multi-function measuring instrument, incl. store for up to 500,000 readings, VAC module (volume flow measurement with error calculation), battery, Li cell and calibration protocol (Part no. 0563 4001)
- ComSoft 3 Professional with data management (Part no. 0554 0830)
- RS232 cable (Part no. 0409 0178)
- Bendable vane probe (can be bent by 90°), Ø 100 mm, attachable to handle 0430 3545 or telescopic handle 0430 0941, for measurements on ventilation outlets (Part no. 0635 9340)
- Vane/temperature probe, Ø 16 mm, attachable to 0430 3545 handle or 0430 0941 telescopic handle (Part no. 0635 9540)
- Professional telescopic handle for plug-in vane probes, max. 1 m long (Part no. 0430 0941)
- Attachable printer (securely attached) including 1 roll of thermal paper and batteries (Part no.
- SoftCase (protects instrument from impact) with carrier strap, magnetic holder and probe holder (Part no. 0516 0401)
- SoftCase for attachable printer (protects printer from dirt/impact) (Part no. 0516 0411)
- System case (aluminium) for measuring instrument, probes and accessories (Part no. 0516 0410)

We recommend:

DAkkS calibration certificate/temperature * 0520 0201 El. resistance thermometer, el. thermometer; cal. points selectable from -80 to +1000°C

The pro set for assessing workplaces subjected to heat

- testo 400, multi-function measuring instrument, incl. store for up to 500,000 readings, VAC module (volume flow measurement with error calculation), battery, Li cell and calibration protocol (Part no. 0563 4001)
- Wet Bulb Globe temperature probe to assess workplaces subjected to heat, in accordance with ISO 7243 or DIN 33403, incl. WBGT case (Part no. 0635 8888)
- Attachable printer (securely attached) including 1 roll of thermal paper and batteries (Part no. 0554 0570)

We recommend:

ISO calibration certificate/temperature for air/immersion probes, calibration points -8°C; 0°C; +40°C 0520 0181

testo 400, the Pro set for comfort level meas. & occupational safety/health

- testo 400 multi-function measuring instrument, incl. store for up to 500,000 readings, VAC module (volume flow measurement with error calculation), battery, Li cell and calibration protocol (Part no. 0563 4001)
- Comfort level probe for measuring degree of turbulence, with telescopic handle and stand. Fulfills EN 13779 requirements (Part no. 0628 0009)
- Attachable printer (securely attached) including 1 roll of thermal paper and batteries (Part no. 0554 0570)

We recommend:

CO2 probe measures indoor air quality and monitors the workplace. With 0632 1240 plug-in head, connection cable 0430 0143 or 0430 0145 required

Cable, 1.5 m long, connects probe with plug-in head to meas. instrument 0430 0143 PUR coating material Standard ambient air probe up to +70°C 0636 9740

Measures all physical parameters in the psychrometric chart Quick-action surface probe with sprung thermocouple strip, measuring 0604 0194 range short-term to +500 °C

Cable, 1.5 m long, connects probe with plug-in head to meas. instrument 0430 0143 PUR coating material

Recommended set

Laboratory fume cupboard probe

- testo 400, multi-function measuring instrument, incl. store for up to 500,000 readings, VAC module (volume flow measurement with error calculation), battery, Li cell and calibration protocol (Part no. 0563 4001)
- Mains unit 230 V/ 8 V/ 1 A, for instrument (European plug) (Part no. 0554 1084)
- Rech. batt, set for instr. (2 rech. 2.4V/1100mAh) (Part no. 0554 0196)
- Thermal anemometer probe, Ø 10 mm, w. telescopic handle, measures air flow in lab fume cupboards to DIN EN 14175 (Part no. 0635 1047)
- Standard ambient air probe up to +70°C (Part no. 0636 9740)
- Pressure probe, 2000 hPa, measures absolute pressure, in robust metal housing with impact protection, incl. quick-closing coupling (M8 x 0.5), magnet for fast attachment (Part no. 0638
- Precision pressure probe, 100 Pa, in robust metal housing with impact protection, incl. magnet for fast attachment, to measure differential pressure and flow speeds (in combination with Pitot tube) (Part no. 0638 1347)
- Cable, 1.5 m long, connects probe with plug-in head to meas. instrument (Part no. 0430 0143)
- Comfort level probe for measuring degree of turbulence, with telescopic handle and stand. Fulfills EN 13779 requirements (Part no. 0628 0009)

We recommend:

ComSoft 3 - Professional with data management incl. database, analysis and graphics function, data analysis, trend curve	0554 0830
RS232 cable connects instrument to PC (1.8 m) for data transfer	0409 0178
Attachable printer (securely attached) including 1 roll of thermal paper and batteries	0554 0570
SoftCase (protects instrument from impact) with carrier strap, magnetic holder and probe holder	0516 0401
SoftCase for attachable printer (protects printer from dirt/impact) protects from impact and falls	0516 0411
System case (aluminium) for measuring instrument, probes and accessories probes in lid make it easy to find parts in case	0516 0410

DAkkS calibration certificate/velocity for laboratory fume cupboard probe*

ISO calibration certificate/velocity for laboratory fume cupboard probe

The Pro Set for clean room systems

- testo 400, multi-function measuring instrument, incl. store for up to 500,000 readings, VAC module (volume flow measurement with error calculation), battery, Li cell and calibration protocol (Part no. 0563 4001)
- Precision pressure probe, 100 Pa, in robust metal housing with impact protection, incl. magnet for fast attachment, to measure differential pressure and flow speeds (in combination with Pitot tube) (Part no. 0638 1347)
- Precision air probe (Part no. 0628 0017)
- Highly accurate reference humidity/temp. probe (Part no. 0636 9741)
- Cable, 1.5 m long, connects probe with plug-in head to meas. instrument (Part no. 0430 0143)
- Cable, 1.5 m long, connects probe with plug-in head to meas. instrument (Part no. 0430 0143)
- Quick-action hot wire probe, Ø 10 mm, with telescopic handle, for measurements in the lower velocity range with direction recognition (Part no. 0635 1041)
- Bendable vane probe (can be bent by 90°), Ø 100 mm, attachable to handle 0430 3545 or telescopic handle 0430 0941, for measurements on ventilation outlets (Part no. 0635 9340)
- Professional telescopic handle for plug-in vane probes, max. 1 m long (Part no. 0430 0941)
- Current/voltage cable (±1 V, ±10 V, 20 mA) (Part no. 0554 0007)
- System case (aluminium) for measuring instrument, probes and accessories (Part no. 0516-0410).
- ComSoft 3 Professional with data management (Part no. 0554 0830)
- RS232 cable (Part no. 0409 0178)

We recommend:

DAkkS calibration certificates for temperature, humidity, velocity, pressure *(See Calibration)

*Successor organization of the DKD



Accessories and calibration certificates

Accessories	Part no.
Accessories for measuring instrument	
Rech. batt. set for instr. (2 rech. 2.4V/1100mAh) elected for quick recharging in instrument	0554 0196
Aains unit 230 V/ 8 V/ 1 A, for instrument (European plug) or mains operation and battery recharging	0554 1084
ithium battery button cell, CR2032 AA batteries for radio handle	0515 0028
Printer and Accessories	
attachable printer (securely attached) including 1 roll of thermal paper and latteries	0554 0570
esto fast printer with wireless infrared interface, 1 roll thermal paper and 4 \upMedsize{A} batteries	0554 0549
ast testo 575 printer, incl. 1 roll of thermal paper and batteries nfrared thermal line printer with graphics function	0554 1775
xternal fast charger for 1-4 AA rech. batteries, incl. 4 Ni-MH rech. batteries with individual cell charging and charge control display, incl. impulse trickle rharging, integrated discharge function, with built-in international mains slug, 100-240 V, 300 mA, 50/60 Hz	0554 0610
Spare thermal paper for printer (6 rolls)	0554 0569
pare thermal paper for printer (6 rolls), permanent ink neasurement data documentation legible for up to 10 years	0554 0568
abel thermal paper (Testo patent) for testo 575 printer (6 rolls), can be pplied directly	0554 0561
SoftCase for instrument and printer	
oftCase (protects instrument from impact) with carrier strap, magnetic older and probe holder	0516 0401
oftCase for attachable printer (protects printer from dirt/impact) rotects from impact and falls	0516 0411
Software and Accessories	
ComSoft 3 - Professional with data management ncl. database, analysis, and graphics function, data analysis, trend curve	0554 0830
IS232 cable onnects instrument to PC (1.8 m) for data transfer	0409 0178
thernet adapter, RS232 - Ethernet incl. software driver, mains unit acilitates data communication in network	0554 1711
System case	
system case (plastic) for measuring instrument, probes and accessories robes in lid make it easy to find parts in case (540 x 440 x 130 mm)	0516 0400
System case (aluminium) for measuring instrument, probes and accessories	0540 0440

for air/immersion probes, calibration points -18°C; 0°C; +60°C SO calibration certificate/remperature Meas. instr. with air/immersion probe; cal. points 0°C; +150°C; +300°C SO calibration certificate/remperature meas. instr. with surface probe; calibration points +60°C; +120°C; +180°C DAkkS calibration certificate/remperature* 0520 0211 meas. instr. with surface probe; calibration points +60°C; +120°C; +180°C DAkkS calibration certificate/remperature* 0520 0211 meas. instr. with air/immersion probe; calibration points -20°C; 0°C; +60°C DAkkS calibration certificate/remperature* 0520 0211 DAkkS calibration certificate/remperature* 0520 0210 Calibration certificate/humidity 0520 0106 SO calibration certificate/humidity 0520 0006 Calibration certificate/humidity 0520 0006 Calibration certificate/humidity 0520 0006 Calibration certificate/humidity 0520 0136 Calibration certificate/humidity 0520 0138 Calibration certificate/humidity 0520 0013 Saturated saline solutions, calibration point 75.3%RH DAkkS calibration certificate/humidity 0520 0206 Calibration certificate/humidity 0520 0208 Calibration certificate/humidity 0520 0208 Calibration certificate/humidity 0520 0213 Calibration certificate/humidity 0520 0213 Calibration certificate/humidity 0520 0225 Calibration certificate/pressure 0520 0213 Calibration certificate/pressure 0520 0225 Calibration certificate/pressure 0520 0215 Calibration certificate/pressure 0520 0215 Calibration certificate/pressure 0520 0215 Calibration certificate/pressure 0520 0215 Calibration certificate/pressure 0520 0216 Calibration cert	Calibration Certificates	Part no.
for air/immersion probes, calibration points -18°C; 0°C; +60°C SO calibration certificate/remperature Meas. Instr. with air/immersion probe; cal points 0°C; +150°C; +300°C ISO calibration certificate/remperature meas. instr. with surface probe; calibration points +60°C; +120°C; +180°C DAkkS calibration certificate/remperature* 0520 0211 DAkkS calibration certificate/remperature* 0520 0271 DAkkS calibration certificate/remperature* 0520 0271 Contact surface temperature probes; calibration points +20°C; 0°C; +60°C DAkkS calibration certificates/humidity SO calibration certificate/humidity SO calibration certificate/humidity SO calibration certificate humidity 0520 0006 Calibration points 1-13. %RH and 75.3 %RH at +25°C SO calibration certificate dewpoint woo adjustment points -10'-40 °Ctd at 6 bar SO calibration certificate formidity 0520 003 SO calibration certificate/humidity 0520 003 SO calibration certificate/humidity 0520 0083 saturated saline solutions: calibration point 75.3%RH DAkkS calibration certificate/humidity 0520 0083 saturated saline solutions: calibration point 75.3%RH DAkkS calibration certificate/humidity 0520 0216 Calibration certificate/humidity 0520 0220 DAkkS calibration certificate/humidity 0520 023 DAkkS calibration certificate/humidity 0520 0216 Calibration certificate/humidity 0520 023 Solution certificate/humidity 0520 023 Solution certificate/humidity 0520 024 Calibration certificate/pressure 0520 025 DAkkS calibration certificate/pressure 0520 025 Calibration certificate/pressure 0520 026 DAkkS calibration certificate/pressure 0520 026 DAkkS calibration certificate/pressure 0520 027 DAkkS calibration certificate/pressure 0520 025 differential pressure, 5 points distributed over meas. range 0520 025 differential pressure, 5 points distributed over meas. range 0520 0215 differential pressure, 5 points distributed over meas. range 0520 0215 DAkkS calibration certificate/pressure 0520 0225 differential pressure, 5 points distributed over meas. range 052	Calibration certificates/temperature	
Meas. instr. with air/immersion probe; cal. points 0°C; +150°C; +300°C SO calibration certificate/remperature meas. Instr. with surface probe; calibration points +60°C; +120°C; +180°C DAkkS calibration certificate/remperature* meas. instr. with surface probe; calibration points +60°C; +120°C; 0°C; +60°C DAkkS calibration certificate/remperature* meas. instr. with air/immersion probe; calibration points +20°C; 0°C; 0°C; +60°C DAkkS calibration certificates/remperature* 0520 0271 contact surface temperature probes; calibration points +100°C; +200°C; +300°C Calibration certificates/humidity SO calibration certificates/humidity 0520 0106 cal. points freely selectable from 5 to 95%RH at +15 to +35°C or at -18 to +80°C ISO calibration certificate humidity 0520 0136 ISO calibration certificate dewpoint 0520 0136 ISO calibration certificate dewpoint 1SO calibration certificate form 5 to 95%RH at +25°C SO calibration certificate/humidity 0520 0033 Socialbration certificate/humidity 0520 0083 Socialbration certificate/humidity 0520 0083 Socialbration certificate/humidity 0520 0083 Socialbration certificate/humidity 0520 0206 electronic hygrometers; calibration points 11.3%RH at +25°C DAkKS calibration certificate/humidity 0520 0216 calibration certificate/humidity 0520 0213 saturated saline solutions; calibration point 11.3%RH DAkKS calibration certificate/humidity 0520 0213 saturated saline solutions; calibration point 11.3%RH DAkKS calibration certificate/humidity 0520 0213 saturated saline solutions; calibration point 17.3%RH Calibration certificate/pressure Socialbration certificate/pressure Socialbrat	ISO calibration certificate/temperature for air/immersion probes, calibration points -18°C; 0°C; +60°C	0520 0001
meas. instr. with surface probe; calibration points +60°C; +120°C; +180°C DAKKS calibration certificate/remperature* meas. instr. with air/immersion probe; calibration points -20°C; 0°C; +60°C DAKKS calibration certificate/remperature* CODAKKS calibration certificate/remperature* CODAKKS calibration certificates/humidity SIO calibration certificates/humidity SIO calibration certificates/humidity SIO calibration certificate humidity Cal. points freely selectable from 5 to 95%RH at +15 to +35°C or at -18 to +80°C SIO calibration certificate humidity Calibration certificate humidity Calibration certificate humidity SIO calibration certificate humidity SIO calibration certificate humidity SIO calibration certificate/humidity SIO calibration certificate/pressure SIO calibration certificate/soloty SIO calibration certificate/soloty SIO calibration cert	ISO calibration certificate/temperature Meas. instr. with air/immersion probe; cal. points 0°C; +150°C; +300°C	0520 0021
meas. instr. with air/immersion probe; calibration points -20°C; 0°C; +60°C DAkkS calibration certificate/temperature* 0520 0271 contact surface temperature probes; calibration points +100°C; +200°C; +300°C Calibration certificates/humidity ISO calibration certificates/humidity ISO calibration certificate humidity ISO calibration certificate humidity Calibration certificate humidity Calibration certificate humidity Calibration certificate dewpoint Wo adjustment points -10/-40 °Ctd at 6 bar ISO calibration certificate/humidity SISO calibration certificate/humidity DAkkS calibration certificate/humidity* DAkkS calibration certificate/humidity* O520 0206 DAkkS calibration certificate/humidity* O520 0213 DAkkS calibration certificate/humidity* O520 0213 DAkkS calibration certificate/humidity* O520 0213 Saturated saline solutions; calibration point 11.3%RH DAkkS calibration certificate/humidity* O520 0283 Saturated saline solutions; calibration point 75.3%RH Calibration certificate/numidity* O520 0283 Saturated saline solutions; calibration point 75.3%RH Calibration certificate/pressure O520 0205 DAkkS calibration certificate/pressure* O520 0205 O520 0225 differential pressure; 5 points distributed over meas. range DAkkS calibration certificate/pressure* O520 0225 differential pressure; 1 measuring points distributed over meas. range DAkkS calibration certificate/pressure* O520 0225 differential pressure; 1 measuring points distributed over the instr. meas. range SO calibration certificate/pressure* O520 0215 differential pressure; 1 measuring points distributed over meas. range Calibration certificate/pressure* O520 0212 DAkkS calibration certificate/pressure* O520 0212 DAkkS calibration certificate/pressure* O520 0212 DAkkS calibration certificate/pressure* O520 0204 To t	ISO calibration certificate/temperature meas. instr. with surface probe; calibration points +60°C; +120°C; +180°C	0520 0071
Calibration certificates/humidity Sign calibration certificate humidity Calibration certificate humidity Sign calibration certificate humidity Calibration points 11.3 %RH and 75.3 %RH at +25°C Sign calibration certificate dewpoint Sign calibration certificate dewpoint Sign calibration certificate/humidity Dakks calibration certificate/humidity Sign calibration certificate/humidity Dakks calibration certificate/humidity Sign cali	DAkkS calibration certificate/temperature* meas. instr. with air/immersion probe; calibration points -20°C; 0°C; $+60$ °C	0520 0211
ISO calibration certificate/humidity call points freely selectable from 5 to 95%RH at +15 to +35°C or at -18 to +80°C SISO calibration certificate humidity Calibration points 11.3 %RH and 75.3 %RH at +25°C SISO calibration certificate dewpoint two adjustment points -10/-40 °Ctd at 6 bar SISO calibration certificate/humidity saturated saline solutions: calibration point 11.3 %RH SISO calibration certificate/humidity saturated saline solutions, calibration point 75.3 %RH DAKKS calibration certificate/humidity* 0520 0208 saturated saline solutions, calibration point 75.3 %RH DAKKS calibration certificate/humidity* 0520 0206 electronic hygrometers; calibration point 51.3 %RH and 75.3 %RH at +25°C DAKKS calibration certificate/humidity* 0520 0216 cal. points freely selectable from 5 to 95%RH at +25°C or -18°C to +70°C DAKKS calibration certificate/humidity* 0520 0213 saturated saline solutions; calibration point 75.3 %RH DAKS calibration certificate/humidity* 0520 0213 saturated saline solutions; calibration point 75.3 %RH Calibration certificate/pressure SISO calibration certificate/pressure SISO calibration certificate/pressure 0520 0225 diff. and pos. pressure; 5 points distributed over meas. range DAKKS calibration certificate/pressure 0520 0225 diff. and pos. pressure; 6 meas. points distributed over meas. range (>0.6% of fsv) DAKS calibration certificate/pressure 0520 0225 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range SISO calibration certificate/pressure* 0520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range SISO calibration certificate/pressure* 0520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range SISO calibration certificate/pressure* 0520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range SISO calibration certificate/pressure* 0520 0212 dalibration certificate/sisolute pressure, 5 measurement points distributed 0520 0212 dalibration certificate/sis	DAkkS calibration certificate/temperature* contact surface temperature probes; calibration points +100°C; +200°C; +3	
cal. points freely selectable from \$\tilde{5}\$ to 95\%RH at +15 to +35\%C or at -18 to +80\%C is Calibration certificate humidity	Calibration certificates/humidity	
Calibration points 11.3 %RH and 75.3 %RH at +25°C ISO calibration certificate dewpoint two adjustment points -10/-40 °Ctd at 6 bar ISO calibration certificate/humidity 0520 0013 Saturated saline solutions, calibration point 11.3 %RH ISO calibration certificate/humidity 0520 0083 saturated saline solutions, calibration point 75.3 %RH DAkkS calibration certificate/humidity* 0520 0206 electronic hygrometers; calibration points 11.3 %RH and 75.3 %RH at +25°C DAkkS calibration certificate/humidity* 0520 0216 cal. points freely selectable from 5 to 95 %RH at +25°C or -18°C to +70°C DAkkS calibration certificate/humidity* 0520 0213 saturated saline solutions; calibration point 11.3 %RH DAkkS calibration certificate/humidity* 0520 0213 saturated saline solutions; calibration point 11.3 %RH Calibration certificate/humidity* 0520 0283 saturated saline solutions; calibration point 75.3 %RH Calibration certificate/pressure ISO calibration certificate/pressure ISO calibration certificate/pressure O520 0005 differential pressure, 5 points distributed over meas. range (>0.6% of fsv) DAkkS calibration certificate/pressure* 0520 0215 differential pressure, accuracy 0.1 to 0.6 (% of fsv) DAkkS calibration certificate/pressure* 0520 0215 differential pressure, 11 measuring points distributed over the instr. meas. range ISO calibration certificate/pressure* 0520 0215 differential pressure, 5 meas. points distributed over the instr. meas. range ISO calibration certificate/pressure* 0520 0212 dabolute pressure, 11 measuring points distributed over meas. range Calibration certificate/pressure* 0520 0212 dabolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAkkS calibration certificate/velocity O520 0004 to ver meas. range Calibration certificate/velocity O520 0004 to ver meas. range Calibration certificate/velocity O520 0004 to ver wea anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s DAkkS calibration certificate/velocity* 0520 0024 hot wire, vane anemometer; calibration points 0.5; 1;	ISO calibration certificate/humidity cal. points freely selectable from 5 to 95%RH at +15 to +35°C or at -18 to + $^{-18}$ to	
two adjustment points -10/-40 °Ctd at 6 bar ISO calibration certificate/humidity saturated saline solutions: calibration point 11.3%RH ISO calibration certificate/humidity saturated saline solutions; calibration point 75.3%RH DAKKS calibration certificate/humidity* electronic hygrometers; calibration points 11.3%RH and 75.3%RH at +25°C DAKKS calibration certificate/humidity* oS20 0216 cal. points freely selectable from 5 to 95%RH at +25°C or -18°C to +70°C DAKKS calibration certificate/humidity* oS20 0213 saturated saline solutions; calibration point 11.3%RH DAKKS calibration certificate/humidity* oS20 0283 saturated saline solutions; calibration point 75.3%RH Calibration certificates/pressure ISO calibration certificate/pressure O520 0005 ISO calibration certificate/pressure O520 0025 differential pressure; 5 points distributed over meas. range DAKKS calibration certificate/pressure O520 0025 differential pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over meas. range ISO calibration certificate/pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure O520 0212 absolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/pressure O520 00125 O520 00126 Calibration certificate/pressure O520 00127 DAKKS calibration certificate/pressure O520 00126 DAKKS calibration certificate/pressure O520 00127 DAKKS calibration certificate/pressure O520 0014 DAKKS calibration certificate/velocity O520 0024 hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration cer	ISO calibration certificate humidity Calibration points 11.3 %RH and 75.3 %RH at +25°C	0520 0006
saturated saline solutions: calibration point 11.3%RH ISO calibration certificate/humidity saturated saline solutions, calibration point 75.3%RH DAKKS calibration certificate/humidity* cal. points freely selectable from 5 to 95%RH at +25°C DAKKS calibration certificate/humidity* cal. points freely selectable from 5 to 95%RH at +25°C or -18°C to +70°C DAKKS calibration certificate/humidity* cal. points freely selectable from 5 to 95%RH at +25°C or -18°C to +70°C DAKKS calibration certificate/humidity* asturated saline solutions; calibration point 11.3%RH DAKKS calibration certificate/humidity* asturated saline solutions; calibration point 75.3%RH Calibration certificate/pressure ISO calibration certificate/pressure SDS calibration certificate/pressure O520 0005 differential pressure; 5 points distributed over meas. range DAKKS calibration certificate/pressure o520 0025 differential pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range SO calibration certificate/pressure, 5 measurement points distributed over the solution certificate/pressure; 5 points distributed over meas. range SO calibration certificate/pressure, 5 measurement points distributed over the instr. meas. range SO calibration certificate/pressure, 5 measurement points distributed over meas. range Calibration certificate/velocity DAKKS calibration certificate/velocity SO calibration certificate/velocity alt velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificates/velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s DAKKS calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s DAKKS calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* bDAKKS calibration certificate/velocity* bDAKKS	ISO calibration certificate dewpoint two adjustment points -10/-40 °Ctd at 6 bar	0520 0136
DAKKS calibration certificate/humidity* O520 0206 electronic hygrometers; calibration points 11.3%RH and 75.3%RH at +25°C DAKKS calibration certificate/humidity* cal. points freely selectable from 5 to 95%RH at +25°C or -18°C to +70°C DAKKS calibration certificate/humidity* cal. points freely selectable from 5 to 95%RH at +25°C or -18°C to +70°C DAKKS calibration certificate/humidity* Saturated saline solutions; calibration point 11.3%RH DAKKS calibration certificate/humidity* O520 0283 Saturated saline solutions; calibration point 75.3%RH Calibration certificate/pressure ISO calibration certificate/pressure SO calibration certificate/pressure offife meas. points distributed over meas. range DAKKS calibration certificate/pressure offife meas. points distributed over meas. range offife medial pressure; 6 meas. points distributed over meas. range offife medial pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* O520 0225 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range over meas. range ISO calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range over meas. range DAKKS calibration certificate/pressure* O520 0215 O520 0212 DAKKS calibration certificate/pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/velocity ISO calibration certificate/velocity o520 0004 all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s DAKKS calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10 m/s DAKKS calibration certificate/velocity* DAKKS calibration certificate/velocity* DAKKS calibration certificate/velocity*	ISO calibration certificate/humidity saturated saline solutions: calibration point 11.3%RH	0520 0013
electronic hygrometers; calibration points 11.3%RH and 75.3%RH at +25°C DAkkS calibration certificate/humidity* cal. points freely selectable from 5 to 95%RH at +25°C or -18°C to +70°C DAkKS calibration certificate/humidity* saturated saline solutions; calibration point 11.3%RH DAkkS calibration certificate/humidity* saturated saline solutions; calibration point 75.3%RH Calibration certificate/humidity* Sio calibration certificate/pressure Sio calibration certificate/pressure O520 0005 differential pressure; 5 points distributed over meas. range DAkkS calibration certificate/pressure* O520 0025 diff and pos. pressure; 6 meas. points distributed over meas. range (>0.6% of fsv) ISO calibration certificate/pressure* O520 0025 differential pressure, accuracy 0.1 to 0.6 (% of fsv) DAkkS calibration certificate/pressure* O520 0215 diff and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range absolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAkkS calibration certificate/pressure* O520 0212 DAkkS calibration certificate/pressure* Calibration certificate/pressure; O520 0212 DAkkS calibration certificate/velocity ISO calibration certificate/velocity of calibration certificate/velocity Not wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s DAkkS calibration certificate/velocity* DAkkS calibration certificate/velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAkkS calibration certificate/velocity hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAkkS calibration certificate/velocity hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAkkS calibration certificate/velocity hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s	ISO calibration certificate/humidity saturated saline solutions, calibration point 75.3%RH	0520 0083
cal. points freely selectable from 5 to 95%RH at +25°C or -18°C to +70°C DAkkS calibration certificate/humidity* saturated saline solutions; calibration point 11.3%RH DAkkS calibration certificate/humidity* 0520 0283 saturated saline solutions; calibration point 75.3%RH Calibration certificates/pressure ISO calibration certificate/pressure* O520 0025 DAkkS calibration certificate/pressure* O520 0025 diff. and pos. pressure; 6 meas. points distributed over meas. range (>0.6% of fsv) ISO calibration certificate/pressure* o520 0025 diff. and pos. pressure; accuracy 0.1 to 0.6 (% of fsv) DAkkS calibration certificate/pressure* o520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range Calibration certificate/absolute pressure* O520 0212 absolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAkkS calibration certificate/velocity SO calibration certificate/velocity SO calibration certificate/velocity all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAkkS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAkkS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAkkS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAkkS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s	DAkkS calibration certificate/humidity* electronic hygrometers; calibration points 11.3%RH and 75.3%RH at +25°C	0520 0206
DAkkS calibration certificate/pressure ISO calibration certificate/pressure O520 0005 Idifferential pressure; 5 points distributed over meas. range DAkkS calibration certificate/pressure* O520 0025 ISO calibration certificate/pressure O520 0025 ISO calibration certificate/pressure O520 0025 ISO calibration certificate/pressure* O520 0025 ISO calibration certificate/pressure* O520 0215 Idiff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range ISO calibration certificate/pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/velocity ISO calibration certificate/velocity ISO calibration certificate velocity ISO calibration certific		0520 0216
Calibration certificates/pressure ISO calibration certificates/pressure ISO calibration certificate/pressure O520 0005 differential pressure; 5 points distributed over meas. range DAKKS calibration certificate/pressure* O520 0025 diff. and pos. pressure; 6 meas. points distributed over meas. range (>0.6% of fsv) ISO calibration certificate/pressure* O520 0025 differential pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/pressure, 5 measurement points distributed over meas. range ISO calibration certificate/pressure, 5 measurement points distributed over meas. range DAKKS calibration certificate/pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/pressure* ISO calibration certificate/velocity ISO calibration certificate/velocity ISO calibration certificate velocity Not wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate velocity Not wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity Not wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s	DAkkS calibration certificate/humidity* saturated saline solutions; calibration point 11.3%RH	0520 0213
ISO calibration certificate/pressure* O520 0005 DAKKS calibration certificate/pressure* O520 0025 differential pressure; 5 points distributed over meas. range DAKKS calibration certificate/pressure* O520 0025 diff and pos. pressure; 6 meas. points distributed over meas. range (>0.6% of fsv) ISO calibration certificate/pressure* O520 0025 differential pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed O520 0125 over meas. range absolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/velocity ISO calibration certificate/velocity all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity*	DAkkS calibration certificate/humidity* saturated saline solutions; calibration point 75.3%RH	0520 0283
DAKKS calibration certificate/pressure* DAKKS calibration certificate/pressure* diff. and pos. pressure; 6 meas. points distributed over meas. range (>0.6% of fsv) ISO calibration certificate/pressure differential pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range absolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/absolute pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/velocity ISO calibration certificate/velocity o520 0104 all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity*		
diff. and pos. pressure; 6 meas. points distributed over meas. range (>0.6% of fsv) ISO calibration certificate/pressure O520 0025 differential pressure, accuracy 0.1 to 0.6 (% of fsv) DAkkS calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed O520 0125 over meas. range absolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAkkS calibration certificate/pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificates/velocity ISO calibration certificates/velocity ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s DAkkS calibration certificate velocity hot wire, vane anemometer, calibration points 0.5; 0.8; 1; 1.5 m/s DAkkS calibration certificate/velocity* O520 0244 hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAkkS calibration certificate/velocity* O520 0204 hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAkkS calibration certificate/velocity* O520 0224 DAkkS calibration certificate/velocity* O520 0224	differential pressure; 5 points distributed over meas. range	
DAKKS calibration certificate/pressure* O520 0215 diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed over meas. range absolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/epressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificate/pressure* O520 0212 absolute pressure; 11 measuring points distributed over meas. range Calibration certificates/velocity ISO calibration certificate/velocity O520 0104 all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate/Velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s	diff. and pos. pressure; 6 meas. points distributed over meas. range (>0.6%	
diff. and pos. pressure; 11 measuring points distributed over the instr. meas. range ISO calibration certificate/absolute pressure, 5 measurement points distributed obver meas. range absolute pressure, a ccuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* absolute pressure; 11 measuring points distributed over meas. range Calibration certificates/velocity ISO calibration certificate/velocity O520 0104 all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity O520 0004 hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate velocity O520 0034 hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity Not wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s		0520 0025
over meas. range absolute pressure, accuracy 0.1 to 0.6 (% of fsv) DAKKS calibration certificate/pressure* absolute pressure; 11 measuring points distributed over meas. range Calibration certificates/velocity ISO calibration certificate/velocity O520 0104 all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity not wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate/Velocity not wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity not wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity not wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* not wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* 0520 0224		
absolute pressure; 11 measuring points distributed over meas. range Calibration certificates/velocity ISO calibration certificate/velocity O520 0104 ISO calibration certificate/velocity O520 0004 ISO calibration certificate velocity Not wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate/Velocity Not wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity Not wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKkS calibration certificate/velocity* Not wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKkS calibration certificate/velocity* Not wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKkS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKkS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKkS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKkS calibration certificate/velocity* Not wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s	over meas, range	0520 0125
ISO calibration certificate/velocity all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity both wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate/Velocity both wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity both wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* both wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* both wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* both wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* both wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* both vire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity*	DAkkS calibration certificate/pressure* absolute pressure; 11 measuring points distributed over meas. range	0520 0212
all velocity probes, calibration points selectable from 0.3 to 50 m/s at +25°C ISO calibration certificate velocity hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate/Velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKkS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKkS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKkS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKkS calibration certificate/velocity* 0520 0224	Calibration certificates/velocity	
hot wire, vane anemometer, Pitot tube; calibration points 1; 2; 5; 10 m/s ISO calibration certificate/Velocity hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* 0520 0224		
hot wire, vane anemometer, Pitot tube; calibration points 5; 10; 15; 20 m/s ISO calibration certificate velocity hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKKS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKKS calibration certificate/velocity* 0520 0224		0520 0004
hot wire, vane anemometer; calibration points 0.5; 0.8; 1; 1.5 m/s DAKkS calibration certificate/velocity* hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAKkS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAKkS calibration certificate/velocity* 0520 0224		0520 0034
hot wire, vane anemometer; calibration points 0.5; 1; 2; 5; 10 m/s DAkkS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAkkS calibration certificate/velocity* 0520 0224		0520 0024
hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s DAkkS calibration certificate/velocity* 0520 0224		0520 0244
	DAkkS calibration certificate/velocity* hot wire, vane anemometer, Pitot tube; calibration points 2; 5; 10; 15; 20 m/s	
		0520 0224

^{*}Successor organization of the DKD



Technical data

Probe type	Vane	Thermal	Testo humid. sensor, cap.	Pressure	aw value
Meas. range	0 to +60 m/s	0 to +20 m/s	0 to+100 %RH	0 to +2000 hPa	0 to +1 aW
Accuracy ±1 digit	See probe data for system accuracy	See probe data for system accuracy	See probe data	Probe 0638 1347 Probe 0638 1447 Probe 0638 1547 Probe 0638 1647 Probe 0638 1647 Probe 0638 1747 Probe 0638 1847 ±0.1% of mv Probe 0638 1841 Probe 0638 1941 Probe 0638 2041 Probe 0638 2041 Probe 0638 2141 ±0.2% of mv	See probe data
Resolution	0.01 m/s (for Ø 60/100 mm), 0.1 m/s (for rem. probes)	0.01 m/s (0 to +20 m/s)	0.1 %RH (0 to +100 %RH)	0.001 hPa (Probe 0638 1347) 0.001 hPa (Probe 0638 1447) 0.1 hPa (Probe 0638 1547) 0.1 hPa (Probe 0638 1647) 0.1 hPa (Probe 0638 1747) 0.1 hPa (Probe 0638 1847) 0.01 bar (Probe 0638 1841) 0.01 bar (Probe 0638 1841) 0.01 bar (Probe 0638 1941) 0.01 bar (Probe 0638 2041) 0.01 bar (Probe 0638 2041)	

Probe type	NTC	Pt100	Type K (NiCr-Ni)	Type S (Pt10Rh-Pt)	Type J (Fe-CuNi)
Meas. range	-40 to +150 °C	-200 to +800 °C	-200 to +1370 °C	0 to +1760 °C	-200 to +1000 °C
Accuracy ±1 digit	±0.2 °C (-10 to +50 °C) ±0.4 °C (-40 to -10.1 °C) ±0.4 °C (+50.1 to +150 °C)	±0.1 °C (-49.9 to +99.9 °C) ±(0.1 °C + 0.1% of mv) (remaining range)	±(0.3 °C + 0.1% of mv)	±1 °C (0 to +1760 °C)	±0.4 °C (-150 to +150 °C) ±1 °C (-200 to -150.1 °C) ±1 °C (+150.1 to +1000 °C)
Resolution	0.1 °C (-40 to +150 °C)	0.01 °C (-99.9 to +300 °C) 0.1 °C (-200 to -100 °C) 0.1 °C (+300.1 to +800 °C)	0.1 °C (-200 to +1370 °C)	1 °C (0 to +1760 °C)	0.1 °C (-200 to +1000 °C)

Probe type	CO2 probe	CO probe	Mechanical	Current/voltage measurement	Current/voltage measurement
Meas. range	0 to +1 Vol. % CO ₂ 0 to +10000 ppm CO ₂	0 to +500 ppm CO	20 to 20000 rpm	0 to +20 mA (0554 0007) 0/4 to 20 mA (0554 0528)	0 to +10 V
Accuracy ±1 digit	See probe data	±5% of mv (0 to +500 ppm CO)	±1 digit	±0.04 mA (0 (0554 0007) to +20 mA) See probe (0554 0528) data	±0.01 V (0 to +10 V)
Resolution			1 rpm	0.01 mA (0 to +20 mA)	0.01 V (0 to +10 V)

Oper. temp.	0 to +50 °C
Storage temp.	-25 to +60 °C
Display	LCD, 4 lines
Battery type	1,5 V AA
Battery life	18 h
PC	RS232 interface
Weight	500 g
Material/Housing	ABS
Warranty	3 years
Memory	500.000

Memory space: 1 MB corresponding to approx. 500,000 readings
Other features: automatic probe recognition
Power: Battery/rech. battery, alternatively 8 V mains unit Battery life in continuous operation with 2 T/C probes



Probes Type K (NiCr-Ni)	Illustration	Meas. range	Accuracy	t99	Part no.
Thermocouple, made of fibre-glass insulated thermal pipes, pack of 5	2000 mm Please order adapter 0600 1693 0 0.8 mr	conductors are wrapped	Class 1** r, flat, oval, opposed and covered with fibre-glass together with fibre-glass and soaked with lacque	5 s s, both er,	0644 1109
Quick-action surface probe with sprung thermocouple strip, measuring range short-term to +500 °C	Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	n please order adapter 060 -200 to +300 °C	Class 2**	3 s	0604 0194
Super quick-action surface probe, probe tip at 90° angle, with sprung thermocouple strip	S Conn. Plus-in he	-200 to +300 °C	Class 2** 30 0143 or 0430 0145 required	3 s	0604 0994
Robust surface probe	150 mm 150 mm 0 4 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-200 to +600 °C	Class 1**	25 s	0604 9993
Robust surface probe with sprung thermocouple strip for high temperature range up to +700°C	200 mm O 15 mm	-200 to +700 °C	Class 2**	3 s	0600 0394
Roller surface probe for measurements on rollers and rotating drums, max. circumferential velocity 18 to 400m/min	274 mm 0 33 mm	-50 to +240 °C	Class 2**		0600 5093
Magnetic probe, adhesive power approx. 20 N, with magnets, for measurements on metal surfaces	35 mm Conn.: Fixed cable	-50 to +170 °C	Class 2**		0600 4793
Magnetic probe, adhesive power approx. 10 N, with magnets, for higher temperatures, measures on metal surfaces	75 mm Conn.: Fixed cable	-50 to +400 °C	Class 2**		0600 4893
Adhesive thermocouple, pack of 2, carrier material: aluminium foil	Diameter extension 2 x 0.2 mm, 0.1 mm thick	-200 to +200 °C	Class 1**		0644 1607
Is fixed at the measuring point using conventional adhesives Fast response immersion/penetration probe	<u>'</u>	-200 to +400 °C	Class 1**	3 s	0004.0000
rast response infinersion/penetration probe	Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	200 10 +400 0	Oldoo 1	0.0	0604 0293
Super quick-action immersion/penetration probe for measurements in liquids	0 1.5 mm 0 1.5 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-200 to +600 °C	Class 1**	1 s	0604 0493
Super quick-action immersion/penetration probe for high temperatures	470 mm Ø 1.5 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-200 to +1100 °C	Class 1**	1 s	0604 0593
Super quick-action immersion/penetration probe for measurements in gases and liquids with a low-mass tip	150 mm 20 mm 0 1.4 mm 0 0.5 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-200 to +600 °C	Class 1**	1 s	0604 9794
Robust immersion/penetration probe made of V4A stainless steel, waterproof and oven-proof, e.g. for the food sector	150 mm 0 3.5 mm 0 3 mm	-200 to +400 °C	Class 1**	3 s	0600 2593
Smelting probe for measurements in non-ferrous melting baths, with exchangeable measuring tip (Measurement tip lifetime: up to 500 measurements in aluminium smelter)	1100 mm Conn.: Fixed cable	-200 to +1250 °C	Class 1**	60 s	0600 5993
Spare measuring tip for smelting probe					0363 1712
Pipe wrap probe for pipes up to 2" in diameter	Conn.: Fixed cable	-60 to +130 °C	Class 2**	5 s	0600 4593
Spare meas. head for pipe wrap probe, TC Type K	15 mm	-60 to +130 °C	Class 2**	5 s	0602 0092

^{*}with EEPROM: Precision adjustment for each probe at a measuring point; measuring range limits are saved in probe; t95 extrapolation; surface allowance in surface probe can be adapted to measuring task

^{**} According to standard EN 60584-2, the accuracy of Classes 1 / 2 refer to -40 to +1000/+1200 °C.



Probes Type K (NiCr-Ni)	Illustration	Meas. range	Accuracy	t99	Part no.
Plug-in measuring tip, 750mm long, flexible, for high temperatures, outer casing: stainless steel 1.4541	750 mm 0 3 mm Please order handle with Part no. 0600 5593	-200 to +900 °C	Class 1 [⋆]	4 s	0600 5393
Plug-in measuring tip, 1200 mm long, flexible, for high temperatures, outer casing: stainless steel 1.4541	1200 mm 0 3 mm Please order handle with Part no. 0600 5593	-200 to +900 °C	Class 1*	4 s	0600 5493
Plug-in measuring tip, 550mm long, flexible, for high temperatures, outer casing: Inconel 2.4816	550 mm 0 3 mm Please order handle with Part no. 0600 5593	-200 to +1100 °C	Class 1*	4 s	0600 5793
Plug-in measuring tip, 1030mm long, flexible, for high temperatures, outer casing: Inconel 2.4816	1030 mm 0 3 mm Please order handle with Part no. 0600 5593	-200 to +1100 °C	Class 1*	4 s	0600 5893

Probes Pt100	Illustration	Meas. range	Accuracy	t99	Part no.
Standard air probe	150 mm 0 3 mm 0 9 mm 0 9 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-200 +600 °C	Class A**	75 s	0604 9773
Precision air probe	150 mm	-100 to +400 °C	1/10 Class B (0 to 100°C) 1/5 Class B (rem. range) to EN 60751**	75 s	0628 0017
Robust surface probe	Tiso mm 0.4 mm 0.9 Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-50 to +400 °C	Class B**	40 s	0604 9973
Velcro probe for pipes with diameter of max. 75 mm	280 mm Connt.: Fixed cable	-50 to +150 °C	Class B**	40 s	0628 0019
Standard immersion/penetration probe	200 mm Stainless Steel 0 3 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-200 to +400 °C	Class A**	20 s	0604 0273
Standard immersion/penetration probe	200 mm Nickel 0 3 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-200 to +550 °C	Class A**	20 s	0604 0274
Highly accurate immersion/penetration probe incl. certificate	295 mm Stainless Steel 0 4 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-40 to +300 °C	±0.05 °C (+0.01 to +100 °C) ±(0.05 °C ±0.05% of mv) (-40 to 0 °C) ±(0.05 °C ±0.05% of mv) (+100.01 to +300 °C)	60 s	0614 0240
Highly accurate immersion/penetration probe	200 mm 0 3 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-100 to +400 °C	1/10 Class B (0 to 100°C) 1/5 Class B (rem. range) to EN 60751**	30 s	0628 0015
Flexible precision immersion probe, cable heat-proof up to $+300^{\circ}\text{C}$	1000 mm 50 mm 0 3.5 mm 0 6 mm Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 required	-100 to +265 °C	1/10 Class B (0 to 100°C) 1/5 Class B (rem. range) to EN 60751**	80 s	0628 0016
Robust immersion/penetration probe with sharpened measuring tip, waterproof and oven-proof	150 mm 0 3.5 mm 0 3.5 mm 0 3 mm	-200 to +400 °C	Class A**	30 s	0604 2573

^{*} According to standard EN 60584-2, the accuracy of Class 1 refers to -40 to +1000 °C.

^{**} According to standard EN 60751, the accuracy of Class A and B refer to -200 to +600 °C.

Probes NTC	Illustration			Meas. range	Accuracy t	99	Part no.
Highly accurate air probe for air and gas temperature measurements with bare, mechanically protected sensor	Conn.: Fixed cable	0 9 mm	-0000	-40 to +130 °C	To UNI curve 6	i0 s	0610 9714
Globe thermometer to measure radiant heat	Ø 150 mm			0 to +120 °C	±0.5 °C (0 to +49.9 °C) ±1 °C (+50 to +120 °C)		0554 0670
	Conn.: Fixed cable				Accuracy corresponds to ISO 7243, ISO 7726, D 27726, DIN 33403 requirements	OIN EN	



More probes	Illustration	Meas. range	Accuracy	Part no.
Ambient CO probe, for detecting CO in buildings and rooms	3	0 to +500 ppm CO	$\pm 5\%$ of mv (+100.1 to +500 ppm CO) ± 5 ppm CO (0 to +100 ppm CO)	0632 3331
	Conn.: Fixed cable 1.5 m			
CO2 probe measures indoor air quality and monitors the workplace. With plug-in head, connection cable 0430 0143 or 0430 0145 required	Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 requ	0 +1 00000 ppm CO ₂	\pm (50 ppm CO $_2$ \pm 2% of mv)(0 to +5000 ppm CO $_2$) \pm (100 ppm CO $_2$ \pm 3% of mv)(+5001 to +10000 ppm CO $_2$)	0632 1240
Mechanical rpm probe with plug-in head Included	(att)	20 to 20000 rpm	±1 digit	0640 0340
2 probe tips Ø 8 and Ø 12 mm	Conn.: Plug-in head. connection cable 0430 0143 or 0430 0145 requ	uired		
1 hollow cone Ø 8 mm				
1 surface speed disc Ø 19 mm to measure rotation	onal speed: rpm = rotational speed in mm/s			
Current/voltage cable (±1 V, ±10 V, 20 mA)		0 to +1000 mV 0 to +10 V 0 to +20 mA	±1 mV (0 to +1000 mV) ±0.01 V (0 to +10 V) ±0.04 mA (0 to +20 mA)	0554 0007
4 to 20 mA interface for connection and		0/4 to 20 mA	±0.04 mA	0554 0528
intermittent power supply to transmitters (scaling via hand-held instrument), in robust metal		Channels: 1 channel, transr	mitter connection via terminal board	
nousing with impact protection, incl. magnet for	Conn.: Plug-in head, connection cable	Auxiliary energy output: 18\	V DC ± 20%	
fast attachment	0430 0143 or 0430 0145 required	max. connection load: 30 m	nA	

Accessories	Part no.
Cable, 1.5 m long, connects probe with plug-in head to meas. instrument, PUR coating material	0430 0143
Cable, 5 m long, connects probe with plug-in head to measuring instrument, PUR coating material	0430 0145
extension cable, 5 m long, between plug-in head cable and instrument, PUR coating material	0409 0063
elescopic handle, max. 1 m, for probe with plug-in head, cable: 2.5 m long, PUR coating material	0430 0144
adapter to connect NiCr-Ni thermocouples and probes with open wire ends	0600 1693
landle for plug-in measuring tip	0600 5593
Silicone heat paste (14g), Tmax = +260°C, improves heat transfer in surface probes	0554 0004
Spare measuring tip for smelting probe	0363 1712

More probes						
Humidity probes	Illustration	Meas. range	Accuracy		t99	Part no.
Standard ambient air probe up to +70°C	Ø 12 mm	0 to +100 %RH -20 to +70 °C	±2 %RH (+2 to +98 %RH)	±0.4 °C (-10 to +50 °C) ±0.5 °C (remaining range)	12 s	0636 9740
	Plug-in head. connection cable 0430 0143 or 0430 0145 re	equired				
Duct humidity/temperature probe Telescopic handle 0430 9715, see Ordering data/Accessorie	180 mm	0 to +100 %RH -20 to +70 °C	±2 %RH (+2 to +98 %RH)	±0.4 °C (-10 to +50 °C) ±0.5 °C (remaining range)	12 s	0636 9715
,	Fixed cable					
Thin humidity probe incl. 4 attachable protection caps for	250 mm	0 to +100 %RH	±2 %RH (+2 to +98	±0.4 °C (-10 to +50 °C)	15 s	0636 2130
ambient air measurements, measurements in exhaust air ducts and equilibrium moisture measurements	Ø 4 mm	-20 to +70 °C	%RH)	±0.5 °C (-20 to -10.1 °C) ±0.5 °C (+50.1 to +70 °C)		
	Plug-in head. connection cable 0430 0143 or 0430 0145 required					
Highly accurate reference humidity/temp. probe	Ø 21 mm	0 to +100 %RH -20 to +70 °C	±1 %RH (+10 to +90 %RH)* ±2 %RH (remaining	$\pm 0.2~^{\circ}\text{C}~(+10~\text{to}~+40~^{\circ}\text{C})$ $\pm 0.4~^{\circ}\text{C}~(\text{remaining range})$	12 s	0636 9741
	Plug-in head. connection cable 0430 0143 or 0430 0145 re	equired	range)			
Humidity/temperature probe	Ø 21 mm	0 +100 %RH -20 to +70 °C	±2 %RH (+2 +98 %RH)	±0.4 °C (+0.1 to +50 °C) ±0.5 °C (-20 to 0 °C) ±0.5 °C (+50.1 to +70 °C)	12 s	0636 9742
	Plug-in head. connection cable 0430 0143 or 0430 0145 re	equired		±0.0 0 (±00.1 10 ±70 0)		

^{*} in the temperature range from $+15^{\circ}\text{C}$ to $+30^{\circ}\text{C}$





Suitable probes at a glance

10010 100	Cartable prob	oo at a g	141100				
Probes Process humidity	Illustration		Meas. range	Accuracy		t99	Part no.
Standard pressure dew point probe for measurements in compressed air systems	300 mm Plug-in head, connection cable 043	30 0143 or 0430 0145	0 to +100 %RH -30 to +50 °C tpd	±0.9 °C tpd (+0.1 to +5 ±1 °C tpd (-4.9 to 0 °C ±2 °C tpd (-9.9 to -5 °C ±3 °C tpd (-19.9 to -10 ±4 °C tpd (-30 to -20 °C	tpd) C tpd) C tpd)	300 s	0636 9840
Precision pressure dew point probe for measurements in compressed air systems incl. cert. with test point -40°C tpd	300 mm Plug-in head. connection cable 043		0 to +100 %RH -60 to +50 °C tpd	±0.8 °C tpd (-4.9 to +5 °C tpd (-9.9 to -5 °C tpd (-19.9 to -10 ±3 °C tpd (-29.9 to -20 ±4 °C tpd (-40 to -30 °C tpd (-40 to -3) °C tpd)) °C tpd)	300 s	0636 9841
High humidity level probe w/ heated sensor element, no humidity on sensor	Plug-in head. connection cable 043	300 mm 0 12 mm 30 0143 or 0430 0145	0 to +100 %RH -20 to +85 °C 5 required	±2.5 %RH (0 to +100 %RH)	±0.4 °C (-10 to +50 ±0.5 °C (-20 to -10. ±0.5 °C (+50.1 to +	1 °C)	0636 2142
Robust high temperature/humidity probe up to +180°C	Plug-in head. connection cable 043	300 mm Ø 12 mm 30 0143 or 0430 0145	0 to +100 %RH -20 to +180 °C 5 required	±2 %RH (+2 to +98 %RH)	3 ±0.4 °C (+0.1 to +5 ±0.5 °C (remaining r		0628 0021
Flexible humidity probe (does not retain shape) or measurements in inaccessible places	1500 m Plug-in head. connection cable 043	Ø 12 mm	0 to +100 %RH -20 to +180 °C	±2 %RH (+2 to +98 %RH)	3 ±0.4 °C (+0.1 to +5 ±0.5 °C (-20 to 0 °C ±0.5 °C (+50.1 to +)	0628 0022
						100	
Probes Material and equilibrium moisture	Illustration		Meas. range	Accuracy	2 .0490/40+- 50	*0\ 00 a	Part no.
Flexible humidity probe with mini module for neas. e.g. on material testing rigs, module cable ength 1500mm, probe tip 50x19x7mm	Plug-in head. connection cable 043	30 0143 or 0430 0145	0 to +100 %RH -20 to +125 °C 5 required	±2 %RH (+2 to +98 %RH)	3 ±0.4 °C (-10 to +50 ±0.5 °C (remaining r		0628 0013
Sword probe for measuring humidity and temperature in stacked material	Plug-in head. connection cable 043	320 mm 18 mm x 5 mm	0 to +100 %RH -20 to +70 °C	±2 %RH (+2 to +98 %RH)	3 ±0.4 °C (-10 to +50 ±0.5 °C (-20 to -10. ±0.5 °C (+50.1 to +	1 °Ć)	0636 0340
Robust humidity probe e.g. for measuring aquilibrium moisture or for measurements in exhaust ducts to +120°C	Plug-in head, connection cable 043	300 mm Ø 12 mm	0 to +100 %RH -20 to +120 °C	±2 %RH (+2 to +98 %RH)	3 ±0.4 °C (-10 to +50 ±0.5 °C (remaining r		0636 2140
Material/building moisture cable	Fluy-III lead. Collinection Cable 04.	30 0143 01 0430 0143	0 to 100 k Ohm = 100 to 0 %		Display values in instr display mean: 100 to to 1 very dry		0636 0565
Probes aw value	Illustration		Meas. range	Accuracy		t99	Part no.
aw value set: pressure-tight precision humidity probe with certificate, measurement chamber and 5 sample bowls (plastic)	Reproducibility of aw value ±0.003	3	0 to +1 aW 0 to +100 %RH -20 to +70 °C	±0.01 aW (+0.1 to +0.9 aW) ±0.02 aW (+0.9 to +1 aW)	9 ±0.4 °C (-10 to +50 ±0.5 °C (remaining r		0628 0024
Differential pressure probe	Illustration	Meas. range	Accuracy	Overload S	Static pressure	Zeroing	Part no.
Precision pressure probe, 100 Pa, in robust metal louising with impact protection, incl. magnet for fast ttachment, to measure differential pressure and flow peeds (in combination with Pitot tube)	Plug-in head. connection cable 0430 0143 or 0430 0145 required	0 to +100 Pa	±(0.3 Pa ±0.5% of mv)		00 hPa	to 20 Pa	0638 1347
Pressure probe, 10 hPa, in robust metal housing with mpact protection incl. magnet for fast attachment, to neasure differential pressure and flow speeds (in combination with Pitot tube)	Plug-in head. connection cable 0430 or 0430 0145 required	0 to +10 hPa 0143	±0.03 hPa	50 hPa 1	000 hPa	to 0,4 hPa	0638 1447
ressure probe, 100 hPa, in robust metal housing with mpact protection, incl. magnet for fast attachment, to neasure differential pressure and flow speeds (in ombination with Pitot tube)	Plug-in head. connection cable 0430 0143 or 0430 0145 required	0 to +100 hPa	±0.5% of mv (+20 to +100 hPa) ±0.1 hPa (0 to +20 hPa)	300 hPa 1	000 hPa	to 4 hPa	0638 1547
Pressure probe, 1000 hPa, measures differential pressure, in robust metal housing with impact protection, ncl. quick-closing coupling (M8 x 0.5), magnet for fast tttachment	Plug-in head. connection cable 0430 0143 or 0430 0145 required	0 to +1000 hPa	±1 hPa (0 to 200 hPa) ±0.5% of mv (200 to 1000 hPa)	2000 hPa 1	000 hPa	to 20 hPa	0638 1647
)		0.4- 00000 -0	F hD- (0 t- 0000				

±5 hPa (0 to +2000 hPa)

0 to +2000 hPa

Plug-in head. connection cable 0430 0143 or 0430 0145 required

0638 1847

Pressure probe, 2000 hPa, measures absolute pressure,

in robust metal housing with impact protection, incl. quick-closing coupling (M8 x 0.5), magnet for fast attachment




Relative pressure probes	Illustration	Meas. range	Accuracy	Overload	Zeroing	Part no.
Low pressure probe, refrigerant-proof stainless steel, up to 10 bar		-1 to +10 bar	±1% of fsv Overload 25 bar	25 bar	to 0,1 bar	0638 1741
	Plug-in head, connection cable 0409 0202 required					screw-in thread 7/16" UNF
High pressure probe, refrigerant-proof stainless steel, up to 30 bar		-1 to +30 bar	±1% of fsv Overload 120 bar	120 bar	to 0,3 bar	0638 1841
	Plug-in head, connection cable 0409 0202 required					screw-in thread 7/16" UNF
High pressure probe, refrigerant-proof stainless steel, up to 40 bar		-1 to +40 bar	±1% of fsv Overload 120 bar	120 bar	to 0,4 bar	0638 1941
	Plug-in head, connection cable 0409 0202 required					screw-in thread 7/16" UNF
High pressure probe, refrigerant-proof stainless steel, up to 100 bar		-1 to +100 bar	±1% of fsv Overload 250 bar	250 bar	to 1 bar	0638 2041
	Plug-in head, connection cable 0409 0202 required					Screw-in thread 7/16" UNF
High pressure probe, refrigerant-proof stainless steel, up to 400 bar		-1 to +400 bar	±1% of fsv Overload 600 bar	600 bar	to 4 bar	0638 2141
	Plug-in head, connection cable 0409 0202 required					Screw-in thread 7/16" UNF

Caps for humidity probes	Illustration			Part no.
Metal protection cage, Ø 12 mm for humidity probes, material: stainless steel V4A. Quick adjustment time, robust and temperature-proof. Used when measuring velocities of less than 10 m/s.		Ø 12 mm	0636 9740, 0636 9715	0554 0755
Cap with wire mesh filter, Ø 12 mm			All humidity probes with Ø 12 mm	0554 0757
PTFE sintered filter, Ø 21 mm, PTFE. Not affected by condensation, water-repellent, resistant to corrosive substances. Applications: compressed air measurements, high humidity range continuous measurements), high flow velocities		Ø 21 mm	All humidity probes with Ø 21 mm	0554 0666
Sintered PTFE filter, Ø 12 mm material PTFE. Favourable behaviour in condensation, water repellent, high resistance to aggressive media. Applications: Compressed air measurements, high numidity range (long-term measurements), high flow velocities.		Ø 12 mm	0636 9769, 0636 9740, 0636 9715	0554 0756
PTFE sintered filter, Ø 12 mm, PTFE. Not affected by condensation, water-repellent, resistant to corrosive substances. Applications: compressed air measurements, high humidity range continuous measurements), high flowvelocities		Ø 12 mm	0628 0021, 0628 0022, 0636 2140, 0636 2142	0554 0758
Stainless steel sintered cap, \emptyset 21 mm, can be screwed onto humidity probe. protection in case of high mechanical load and high velocities	E	Ø 21 mm	All humidity probes Ø 21 mm	0554 0640
Stainless steel sintered cap, Ø 12 mm, material: stainless steel V2A. Very rugged, suitable for penetration, can be cleaned with compressed air, mechanical sensor protection. Applications: High mechanical loads, high flow velocities.		Ø 12 mm	0636 9740, 0636 9715	0554 0647
PTFE cap, \emptyset 5 mm, attachable, PTFE material, (5 off). Applications: dust protection, high humidity evel measurements, high flow velocities		Ø 5 mm	0636 2130	0554 1031

Accessories: Humidity probes	Part no.
Cable, 1.5 m long, connects probe with plug-in head to meas. instrument PUR coating material	0430 0143
Cable, $5\mathrm{m}$ long, connects probe with plug-in head to measuring instrument PUR coating material	0430 0145
Extension cable, 5 m long, between plug-in head cable and instrument PUR coating material	0409 0063
Telescopic handle, max. 1 m, for probe with plug-in head cable: 2.5 m long, PUR coating material	0430 0144
Adapter for surface humidity measurement, for humidity probes 0 12 mm locates damp spots on walls, for example	0628 0012
Cap for bore holes, for humidity probe Ø 12 mm Measures equilibrium moisture in bore holes	0554 2140
testo saline pots for control and humidity adjustment of humidity probes, 11.3 %RH and 75.3 %RH with adapter for humidity probe	0554 0660

Accessories: Pressure probes	Part no.
Connection cable, 2.5 m long, for pressure probes 0638 1741/1841/1941	0409 0202
Adapter for pressure probes, 1/2" outer thread, 1/4" inner thread for pressure probes 0638 1741/1841/1941/2041/2141	0699 3127
Cable, 1.5 m long, connects probe with plug-in head to meas. instrument PUR coating material	0430 0143
Cable, 5 m long, connects probe with plug-in head to measuring instrument PUR coating material	0430 0145
Connection hose, silicone, 5m long max. load 700 hPa (mbar)	0554 0440
Connection hose set, 2 x 1 m, coiled, incl. 1/8" screw connection Pressure-tight up to 20 bar, for probe 0638 1647/1747/1847	0554 0441



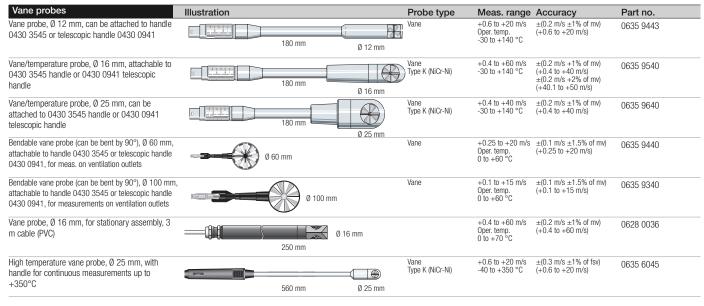

Accessories: Vane probes	Part no.
Professional telescopic handle for plug-in vane probes, max. 1 m long	0430 0941
Extension for telescopic handle, 2 m long please also order the 0409 0063 extension cable	0430 0942
Handle for plug-in vane probes	0430 3545

Thermal probes	Illustration		Probe type	Meas. range	Accuracy	Part no.
Robust hot bulb probe, Ø 3 mm, for measurements in the lower velocity range, 2m cable (PVC)	[\$ \$]	### > Ø3mm	Hot bulb NTC	0 to +10 m/s -20 to +70 °C	±(0.03 m/s ±5% of mv) (0 to +10 m/s)	0628 0035
cable (i vo)	150 mm					
Affordable, robust hot bulb probe, Ø 3 mm, for measurements in the lower velocity range, with			Hot bulb NTC	0 to +10 m/s -20 to +70 °C	±(0.03 m/s ±5% of mv) (0 to +10 m/s)	0635 1549
handle	150 mm	Ø 3 mm				
Robust hot bulb probe, Ø 3 mm, with handle and telescopic handle for measurements in the lower			Hot bulb NTC	0 to +10 m/s -20 to +70 °C	±(0.03 m/s ±5% of mv) (0 to +10 m/s)	0635 1049
velocity range	850 mm	Ø 3 mm				
Quick-action hot wire probe, Ø 10 mm, with telescopic handle, for measurements in the lower			Hot wire NTC	0 to +20 m/s -20 to +70 °C	±(0.03 m/s ±4% of mv) (0 to +20 m/s)	0635 1041
velocity range with direction recognition	760 mm	Ø 10 mm				
Thermal anemometer probe, Ø 10 mm, w. telescopic handle, measures air flow in lab fume			Hot wire NTC	0 to +5 m/s 0 to +50 °C	±(0.02 m/s ±5% of mv) (0 to +5 m/s)	0635 1047
cupboards to DIN EN 14175	760 mm	Ø 10 mm				

Differential pressure probes	Illustration	Probe type	Meas. range	Accuracy	Overload	Static pressure	Zeroing	Part no.
Precision pressure probe, 100 Pa, in robust metal housing with impact protection, incl. magnet for fast attachment, to measure differential pressure and flow speeds (in combination with Pitot tube)	a a	Differential pressure probe	0 to +100 Pa	±(0.3 Pa ±0.5% of mv)	50 hPa	100 hPa	to 20 Pa	0638 1347
Pressure probe, 10 hPa, in robust metal housing with impact protection incl. magnet for fast attachment, to measure differential pressure and flow speeds (in combination with Pitot tube)	R. C.	Differential pressure probe	0 to +10 hPa	±0.03 hPa	50 hPa	1000 hPa	to 0,4 hPa	0638 1447
Pressure probe, 100 hPa, in robust metal housing with impact protection, incl. magnet for fast attachment, to measure differential pressure and flow speeds (in combination with Pitot tube)	A. C.	Differential pressure probe	0 to +100 hPa	±0.5% of mv (+20 t +100 hPa) ±0.1 hPa (0 to +20 hPa)	000 111 0	1000 hPa	to 4 hPa	0638 1547



Suitable probes at a glance

Prandtl's Pitot tubes	Illustration	Accuracy	Part no.
Pitot tube, 300 mm long, stainless steel, for	Ø 4 mm	Oper. temp. 0 to +600 °C	0635 2245
measuring flow velocity		0.0.1000	
	300 mm		
Pitot tube, 350 mm long, \emptyset 7 mm, stainless steel, measures flow speed	Ø 7 mm	Oper. temp. 0 to +600 °C	0635 2145
	350 mm		
Pitot tube, 500 mm long, Ø 7 mm, stainless steel, measures flow speed	[Oper. temp. 0 to +600 °C	0635 2045
modeli ob now opoda			
	500 mm		
Pitot tube, 1000 mm long, stainless steel, measures flow speed	0 7 mm	Oper. temp. 0 to +600 °C	0635 2345
	1000 mm		

Straight Pitot tubes	Illustration			Probe type	Meas. range	Part no.
Pitot tube, stainless steel, 360 mm long, for measuring flow velocity incl.temperature, for pressure probes 0638				Type K (NiCr-Ni)	-40 to +600 °C	0635 2040
1347/1447/1547		360 mm	Ø 8 mm			
Pitot tube, stainless steel, 500 mm long, for measuring flow velocity incl. temperature, for pressure probes 0638				Type K (NiCr-Ni)	-40 to +600 °C	0635 2140
1347/1447/1547		500 mm	Ø 8 mm			
Pitot tube, stainless steel, 1000 mm long, for measuring				Type K (NiCr-Ni)	-40 to +600 °C	0635 2240
flow velocity incl. temperature, for pressure probes 0638 1347/1447/1547		1000 mm	Ø 8 mm			

Accessories: Pressure probes	Part no.
Connection hose, silicone, 5m long max. load 700 hPa (mbar)	0554 0440

Cable, 1.5 m long, connects probe with plug-in head to meas. instrument $\,$ 0430 0143 PUR coating material $\,$

Comfort level measurement	Illustration		Probe type	Meas. range	Accuracy	Part no.
3-function probe for simultaneous measurement of temperature, humidity and velocity. With plug-in head, 0430 0143 connection cable required	270 mm	Ø 21 mm	Hot bulb Testo humid. sensor, cap. NTC	0 to +10 m/s 0 to +100 %RH -20 to +70 °C	±(0.03 m/s ±5% of mv)(0 to 10 m/s) ±2 %RH (+2 to +98 %RH) ±0.4 °C (0 to +50 °C) ±0.5 °C (remaining range)	0635 1540
Comfort level probe for measuring degree of turbulence, with telescopic handle and stand. Fulfills EN 13779 requirements	890 mm		Hot wire NTC	0 to +5 m/s 0 to +50 °C	±(0.03 m/s ±4% of mv) (0 to +5 m/s) ±0.3 °C (0 to +50 °C)	0628 0009
Wet Bulb Globe temperature probe to assess workplaces subjected to heat, in accordance with ISO 7243 or DIN	Ø 150 mm			0 to +120 °C	In accordance with ISO 7243 or DIN 33403	0635 8888
33403, incl. WBGT case					7243 OI DIN 33403	ID No. 0699 4239/1

Accessories: 3-Function probe	Part no.
Cable, 1.5 m long, connects probe with plug-in he PUR coating material	ead to meas. instrument 0430 0143



Notes	





Testo: At Your Service

Please send for more information:

Monitoring Instruments for Food Produ	uction, Transport and Storage
Measurement Engineering for Restaura Supermarkets	ants, Catering and

Measurement Engineering for Air Conditioning and Ventilation

Measurement Engineering for Heating and Installation

Measurement Solutions for Emissions, Service and Thermal Processes

Measurement Solutions for Refrigeration Technology

Stationary Measurement Solutions – Transmitters and Monitoring Systems $\,$

Measurement Solutions for Production, Quality Control and Maintenance

Measurement Solutions for Climate Applications in Industry

Reference Measurement Technology for Industry

Measuring Instruments For Temperature

Measuring Instruments for Humidity

Measuring Instruments For Velocity

Measuring Instruments for Pressure and Refrigeration

Multi-Function Measuring Instruments

Measuring Instruments for Flue Gas and Emissions

Measuring Instruments for RPM, Analysis, Current/Voltage

Measuring Instruments For Indoor Air Quality, Light And Sound

Stationary Measurement Technology Humidity / Differential Pressure / Temperature / Process Displays

Stationary Measurement Technology Compressed Air Humidity / Compressed Air Consumption